

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048101.D
 Acq On : 15 Apr 2022 14:35
 Operator : SY/MD
 Sample : VIBLK060
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rBV	166434	193874	15.61%	1.855%
2	1.916	171	179	198	rVB	128671	180849	14.56%	1.730%
3	2.568	369	382	401	rBV	275264	461097	37.12%	4.411%
4	2.710	421	426	428	rBV3	373	370	0.03%	0.004%
5	2.793	447	452	454	rBV3	622	590	0.05%	0.006%
6	2.961	499	504	510	rVB3	502	663	0.05%	0.006%
7	3.051	524	532	542	rVB3	2651	5179	0.42%	0.050%
8	3.092	542	545	550	rBV2	248	263	0.02%	0.003%
9	3.141	556	560	564	rBV2	231	217	0.02%	0.002%
10	3.195	569	577	581	rBV2	620	918	0.07%	0.009%
11	3.478	661	665	672	rVB3	424	517	0.04%	0.005%
12	3.565	688	692	694	rBV2	296	225	0.02%	0.002%
13	3.678	724	727	731	rVB2	296	240	0.02%	0.002%
14	3.870	783	787	791	rBV3	285	244	0.02%	0.002%
15	3.989	818	824	828	rVB2	286	282	0.02%	0.003%
16	4.121	859	865	868	rBV	274	212	0.02%	0.002%
17	4.562	998	1002	1006	rVB2	307	303	0.02%	0.003%
18	4.629	1006	1023	1072	rBV	113454	306954	24.71%	2.936%
19	4.893	1103	1105	1114	rVB3	370	387	0.03%	0.004%
20	4.931	1114	1117	1119	rBV3	325	228	0.02%	0.002%
21	5.067	1142	1159	1187	rBV	224042	488518	39.33%	4.673%
22	5.192	1196	1198	1201	rVB4	463	295	0.02%	0.003%
23	5.211	1201	1204	1207	rBV4	311	262	0.02%	0.003%
24	5.240	1212	1213	1220	rVV3	313	333	0.03%	0.003%
25	5.288	1225	1228	1238	rVB2	705	845	0.07%	0.008%
26	5.385	1254	1258	1263	rVB3	296	282	0.02%	0.003%
27	5.542	1304	1307	1313	rVV2	299	368	0.03%	0.004%
28	5.729	1342	1365	1388	rBV2	461602	1242129	100.00%	11.882%
29	5.877	1409	1411	1415	rVB3	427	268	0.02%	0.003%
30	6.044	1459	1463	1466	rVB3	539	457	0.04%	0.004%
31	6.066	1466	1470	1474	rVB3	295	225	0.02%	0.002%
32	6.108	1478	1483	1487	rBV4	380	328	0.03%	0.003%
33	6.250	1511	1527	1552	rBV	474018	905524	72.90%	8.662%
34	6.411	1574	1577	1579	rBV2	322	255	0.02%	0.002%
35	6.423	1579	1581	1587	rVB3	513	322	0.03%	0.003%
36	6.536	1605	1616	1622	rBV6	1751	3372	0.27%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048101.D
 Acq On : 15 Apr 2022 14:35
 Operator : SY/MD
 Sample : VIBLK060
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.693	1650	1665	1686	rBV	281156	553888	44.59%	5.298%
38	6.812	1700	1702	1706	rVB3	632	391	0.03%	0.004%
39	7.047	1769	1775	1783	rVB3	486	693	0.06%	0.007%
40	7.108	1789	1794	1800	rBV2	271	440	0.04%	0.004%
41	7.166	1805	1812	1813	rBV	559	464	0.04%	0.004%
42	7.185	1813	1818	1824	rVV3	2177	3179	0.26%	0.030%
43	7.211	1824	1826	1832	rVB3	727	501	0.04%	0.005%
44	7.256	1837	1840	1846	rBV	320	224	0.02%	0.002%
45	7.353	1867	1870	1873	rVB	298	229	0.02%	0.002%
46	7.378	1873	1878	1882	rBV2	486	522	0.04%	0.005%
47	7.568	1919	1937	1961	rBV	143443	257848	20.76%	2.467%
48	7.648	1961	1962	1967	rVB2	595	276	0.02%	0.003%
49	7.690	1967	1975	1983	rBV3	1487	2465	0.20%	0.024%
50	7.767	1995	1999	2005	rVB3	300	319	0.03%	0.003%
51	7.800	2005	2009	2011	rBV2	480	392	0.03%	0.004%
52	7.899	2025	2040	2056	rBV	564314	976664	78.63%	9.343%
53	8.179	2116	2127	2143	rBV	99730	174595	14.06%	1.670%
54	8.259	2149	2152	2154	rBV3	475	373	0.03%	0.004%
55	8.372	2184	2187	2189	rBV3	390	269	0.02%	0.003%
56	8.423	2200	2203	2206	rBV2	296	229	0.02%	0.002%
57	8.455	2208	2213	2215	rBV2	345	295	0.02%	0.003%
58	8.552	2238	2243	2247	rVB3	364	399	0.03%	0.004%
59	8.636	2255	2269	2301	rBV	356812	675438	54.38%	6.461%
60	8.899	2349	2351	2355	rVB2	414	300	0.02%	0.003%
61	9.005	2379	2384	2385	rBV	359	252	0.02%	0.002%
62	9.163	2428	2433	2438	rBV2	485	433	0.03%	0.004%
63	9.417	2499	2512	2547	rBV	718497	1233441	99.30%	11.799%
64	9.632	2575	2579	2580	rBV2	334	223	0.02%	0.002%
65	9.645	2580	2583	2588	rVB3	444	358	0.03%	0.003%
66	9.687	2593	2596	2599	rBV2	433	412	0.03%	0.004%
67	9.796	2627	2630	2634	rBV2	251	254	0.02%	0.002%
68	10.491	2842	2846	2849	rVB	334	228	0.02%	0.002%
69	10.674	2895	2903	2913	rVB2	2539	3591	0.29%	0.034%
70	10.758	2916	2929	2947	rBV	400341	645323	51.95%	6.173%
71	10.867	2959	2963	2969	rVV3	493	533	0.04%	0.005%
72	10.922	2978	2980	2984	rBV	313	235	0.02%	0.002%
73	11.076	3021	3028	3031	rVB3	358	459	0.04%	0.004%
74	11.115	3037	3040	3044	rBV3	474	454	0.04%	0.004%
75	11.153	3048	3052	3055	rVB2	372	293	0.02%	0.003%
76	11.211	3066	3070	3073	rBV4	293	300	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048101.D
 Acq On : 15 Apr 2022 14:35
 Operator : SY/MD
 Sample : VIBLK060
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK060

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.459	3140	3147	3149	rBV3	1340	1523	0.12%	0.015%
78	11.539	3169	3172	3176	rBV	365	262	0.02%	0.003%
79	11.581	3176	3185	3188	rVV3	385	515	0.04%	0.005%
80	11.690	3210	3219	3220	rBV3	750	812	0.07%	0.008%
81	11.751	3232	3238	3245	rBV3	898	1186	0.10%	0.011%
82	11.812	3245	3257	3277	rBV	751109	1203330	96.88%	11.511%
83	11.967	3302	3305	3306	rBV3	825	455	0.04%	0.004%
84	12.018	3319	3321	3325	rVB3	379	245	0.02%	0.002%
85	12.089	3341	3343	3348	rVB2	355	239	0.02%	0.002%
86	12.114	3348	3351	3354	rBV2	434	336	0.03%	0.003%
87	12.195	3360	3376	3396	rBV	529695	895823	72.12%	8.569%
88	12.330	3414	3418	3419	rBV4	483	328	0.03%	0.003%
89	12.459	3456	3458	3465	rVV2	287	318	0.03%	0.003%
90	12.581	3493	3496	3499	rBV3	296	249	0.02%	0.002%
91	12.645	3513	3516	3519	rBV	332	239	0.02%	0.002%
92	13.008	3626	3629	3630	rBV	508	247	0.02%	0.002%
93	13.140	3665	3670	3674	rBV2	489	570	0.05%	0.005%
94	13.848	3881	3890	3902	rBV3	5441	8406	0.68%	0.080%
95	14.336	4036	4042	4050	rVB4	1471	1989	0.16%	0.019%
96	14.536	4102	4104	4107	rVB	480	232	0.02%	0.002%
97	14.590	4117	4121	4125	rBV4	456	470	0.04%	0.004%
98	14.632	4132	4134	4139	rBV3	426	464	0.04%	0.004%
99	15.581	4427	4429	4433	rBV3	621	435	0.04%	0.004%
100	15.677	4456	4459	4460	rBV3	686	453	0.04%	0.004%




Sum of corrected areas: 10453703

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048101.D
Acq On : 15 Apr 2022 14:35
Operator : SY/MD
Sample : VIBLK060
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK060

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

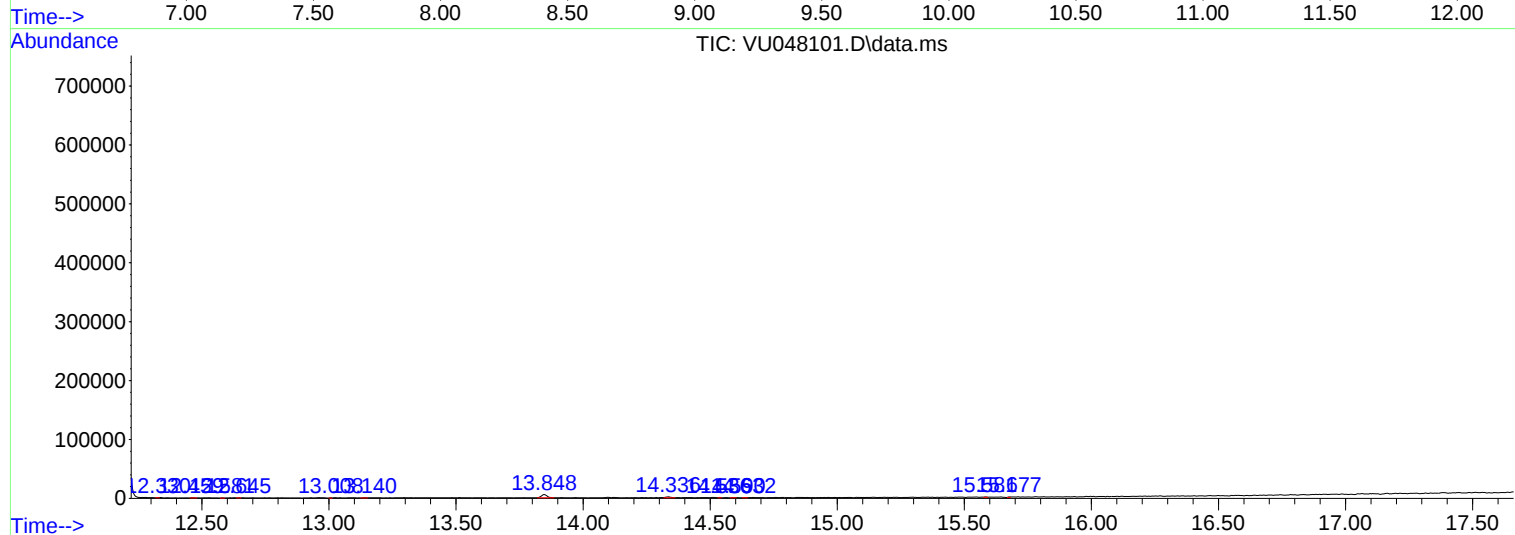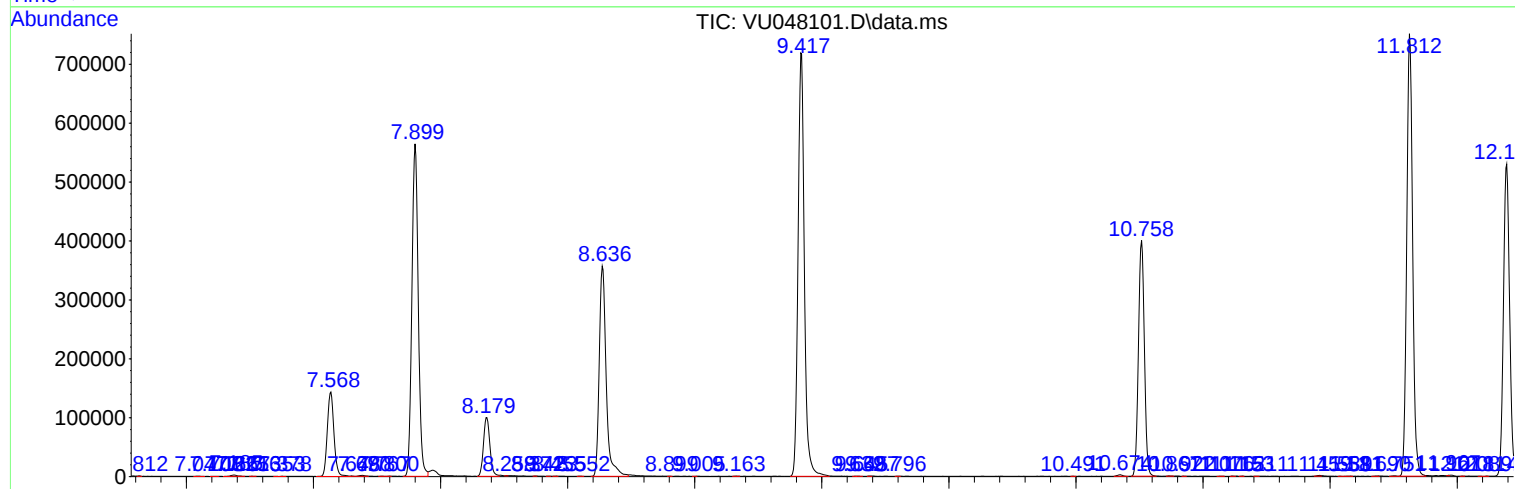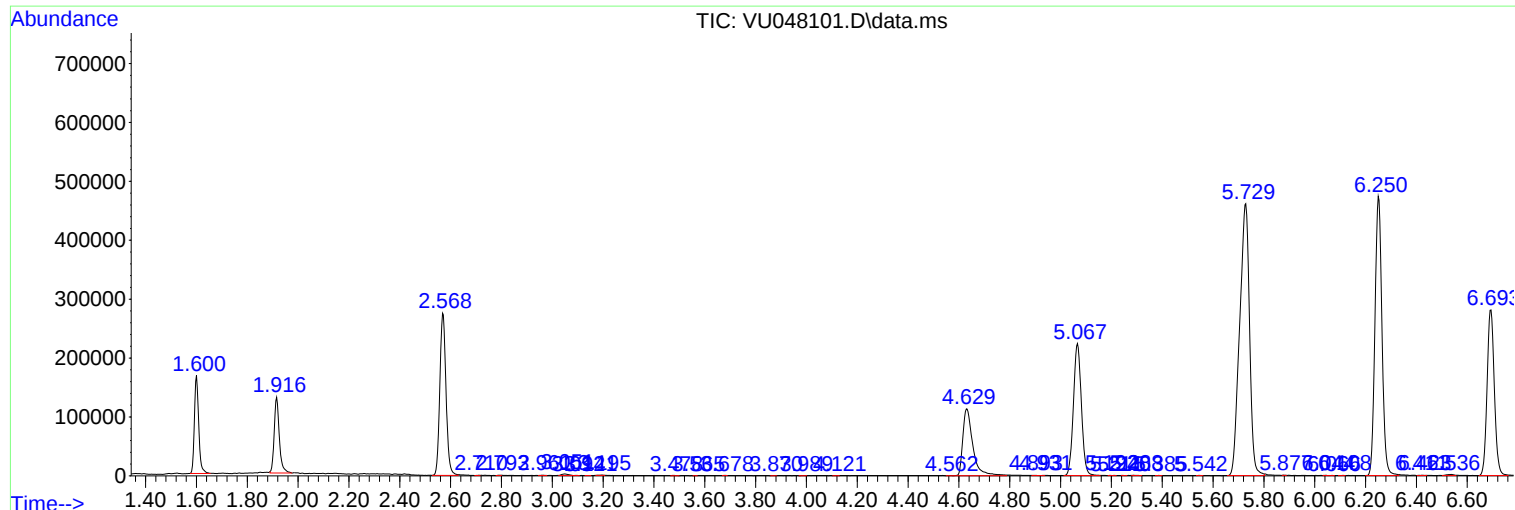

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048101.D
Acq On : 15 Apr 2022 14:35
Operator : SY/MD
Sample : VIBLK060
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK060

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048101.D
Acq On : 15 Apr 2022 14:35
Operator : SY/MD
Sample : VIBLK060
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK060

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------