

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048102.D
 Acq On : 15 Apr 2022 14:58
 Operator : SY/MD
 Sample : N2386-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	53	57	63	rBV3	1916	2426	0.19%	0.023%
2	1.600	74	81	97	rBV	176364	201219	16.15%	1.923%
3	1.916	170	179	199	rVB	125954	179070	14.37%	1.711%
4	2.571	366	383	396	rBV	281482	465744	37.37%	4.451%
5	2.726	428	431	434	rBV3	410	340	0.03%	0.003%
6	2.797	447	453	460	rVB2	1561	1810	0.15%	0.017%
7	3.047	526	531	533	rBV4	620	613	0.05%	0.006%
8	3.189	560	575	593	rBV	15497	34907	2.80%	0.334%
9	3.414	642	645	648	rVB2	357	235	0.02%	0.002%
10	3.433	648	651	653	rBV2	360	249	0.02%	0.002%
11	3.478	662	665	668	rVB3	292	206	0.02%	0.002%
12	3.626	708	711	714	rVB	349	245	0.02%	0.002%
13	3.790	760	762	766	rVB2	395	290	0.02%	0.003%
14	4.022	831	834	839	rVB	313	191	0.02%	0.002%
15	4.321	922	927	930	rVB3	193	209	0.02%	0.002%
16	4.462	967	971	977	rBV3	265	287	0.02%	0.003%
17	4.555	997	1000	1003	rVB	265	185	0.01%	0.002%
18	4.620	1006	1020	1058	rBV2	116401	294919	23.66%	2.819%
19	5.067	1141	1159	1182	rBV	217861	481112	38.60%	4.598%
20	5.224	1204	1208	1211	rVB3	355	213	0.02%	0.002%
21	5.298	1223	1231	1239	rBV2	747	1321	0.11%	0.013%
22	5.507	1293	1296	1301	rBV2	258	296	0.02%	0.003%
23	5.536	1301	1305	1307	rVV	275	217	0.02%	0.002%
24	5.729	1339	1365	1394	rBV2	456593	1233256	98.96%	11.787%
25	5.993	1444	1447	1450	rVB	400	249	0.02%	0.002%
26	6.028	1456	1458	1460	rBV2	379	231	0.02%	0.002%
27	6.054	1464	1466	1469	rVB4	449	228	0.02%	0.002%
28	6.079	1470	1474	1477	rBV	237	235	0.02%	0.002%
29	6.115	1481	1485	1488	rBV3	429	381	0.03%	0.004%
30	6.147	1491	1495	1498	rVB4	420	286	0.02%	0.003%
31	6.185	1502	1507	1512	rVB3	322	303	0.02%	0.003%
32	6.250	1512	1527	1555	rBV	362962	687285	55.15%	6.569%
33	6.526	1609	1613	1617	rBV5	1125	1313	0.11%	0.013%
34	6.597	1633	1635	1638	rBV2	471	237	0.02%	0.002%
35	6.693	1650	1665	1686	rBV	273119	548601	44.02%	5.243%
36	6.767	1686	1688	1693	rVB2	635	507	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048102.D
 Acq On : 15 Apr 2022 14:58
 Operator : SY/MD
 Sample : N2386-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.806	1697	1700	1703	rBV2	619	526	0.04%	0.005%
38	6.857	1713	1716	1718	rBV	307	194	0.02%	0.002%
39	6.886	1718	1725	1726	rBV4	1148	965	0.08%	0.009%
40	7.050	1769	1776	1784	rBV3	328	499	0.04%	0.005%
41	7.160	1801	1810	1811	rVV2	231	278	0.02%	0.003%
42	7.185	1811	1818	1830	rVB4	2015	3548	0.28%	0.034%
43	7.308	1854	1856	1860	rVV2	221	191	0.02%	0.002%
44	7.568	1924	1937	1960	rBV2	142618	255377	20.49%	2.441%
45	7.693	1969	1976	1982	rVB3	1201	1719	0.14%	0.016%
46	7.735	1986	1989	1995	rVB3	368	271	0.02%	0.003%
47	7.899	2025	2040	2056	rBV	558871	961806	77.18%	9.192%
48	8.182	2116	2128	2144	rBV	97238	168902	13.55%	1.614%
49	8.385	2188	2191	2194	rVB2	396	250	0.02%	0.002%
50	8.472	2209	2218	2232	rBV2	2794	4839	0.39%	0.046%
51	8.632	2253	2268	2307	rBV	321196	639021	51.28%	6.107%
52	8.787	2308	2316	2335	rVV3	18023	33248	2.67%	0.318%
53	8.854	2335	2337	2341	rVB4	334	226	0.02%	0.002%
54	9.012	2384	2386	2391	rVV2	295	207	0.02%	0.002%
55	9.092	2408	2411	2415	rVB2	282	228	0.02%	0.002%
56	9.198	2439	2444	2446	rBV2	339	255	0.02%	0.002%
57	9.256	2458	2462	2467	rVB2	237	248	0.02%	0.002%
58	9.285	2467	2471	2473	rBV	266	225	0.02%	0.002%
59	9.369	2492	2497	2499	rBV	208	199	0.02%	0.002%
60	9.417	2499	2512	2555	rVV2	526180	1190754	95.55%	11.380%
61	9.664	2587	2589	2593	rBV3	322	249	0.02%	0.002%
62	9.700	2593	2600	2605	rVV4	992	1236	0.10%	0.012%
63	9.745	2610	2614	2620	rBV3	489	588	0.05%	0.006%
64	9.783	2623	2626	2628	rVV	307	185	0.01%	0.002%
65	9.922	2666	2669	2672	rVB	385	218	0.02%	0.002%
66	10.025	2699	2701	2706	rBV	498	462	0.04%	0.004%
67	10.070	2711	2715	2719	rVV3	328	259	0.02%	0.002%
68	10.198	2752	2755	2759	rVB2	230	198	0.02%	0.002%
69	10.237	2764	2767	2770	rVV2	241	203	0.02%	0.002%
70	10.343	2798	2800	2801	rBV	590	289	0.02%	0.003%
71	10.488	2840	2845	2848	rBV2	212	198	0.02%	0.002%
72	10.674	2894	2903	2912	rVB3	3205	4497	0.36%	0.043%
73	10.758	2916	2929	2953	rVB	397662	647095	51.92%	6.185%
74	10.864	2956	2962	2963	rBV3	428	376	0.03%	0.004%
75	10.896	2965	2972	2973	rBV5	3426	3271	0.26%	0.031%
76	11.005	3000	3006	3014	rVB4	414	662	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048102.D
 Acq On : 15 Apr 2022 14:58
 Operator : SY/MD
 Sample : N2386-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.121	3037	3042	3047	rBV2	683	765	0.06%	0.007%
78	11.192	3058	3064	3065	rBV2	217	201	0.02%	0.002%
79	11.459	3138	3147	3156	rVV5	2223	3372	0.27%	0.032%
80	11.584	3180	3186	3188	rBV2	321	313	0.03%	0.003%
81	11.693	3215	3220	3226	rVB4	1372	1643	0.13%	0.016%
82	11.748	3226	3237	3245	rBV3	43817	69000	5.54%	0.659%
83	11.812	3246	3257	3283	rVB2	590468	1246247	100.00%	11.911%
84	11.944	3293	3298	3302	rBV4	1253	1458	0.12%	0.014%
85	12.069	3328	3337	3348	rBV6	3325	6388	0.51%	0.061%
86	12.195	3362	3376	3398	rBV2	577607	1056791	84.80%	10.100%
87	12.333	3416	3419	3429	rVB6	1071	1241	0.10%	0.012%
88	12.394	3436	3438	3440	rBV3	358	198	0.02%	0.002%
89	12.433	3448	3450	3453	rBV2	357	208	0.02%	0.002%
90	12.481	3462	3465	3467	rBV	452	306	0.02%	0.003%
91	12.597	3497	3501	3502	rBV2	530	295	0.02%	0.003%
92	12.693	3528	3531	3533	rBV2	336	202	0.02%	0.002%
93	12.770	3550	3555	3558	rBV2	869	785	0.06%	0.008%
94	12.918	3596	3601	3604	rBV3	530	445	0.04%	0.004%
95	12.967	3613	3616	3618	rBV2	336	251	0.02%	0.002%
96	13.143	3668	3671	3674	rBV3	317	186	0.01%	0.002%
97	13.757	3859	3862	3870	rVB2	467	482	0.04%	0.005%
98	13.844	3883	3889	3897	rVB3	5180	7426	0.60%	0.071%
99	14.458	4077	4080	4083	rBV	316	232	0.02%	0.002%
100	15.542	4413	4417	4426	rVB5	1121	1313	0.11%	0.013%


Sum of corrected areas: 10463126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048102.D
Acq On : 15 Apr 2022 14:58
Operator : SY/MD
Sample : N2386-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

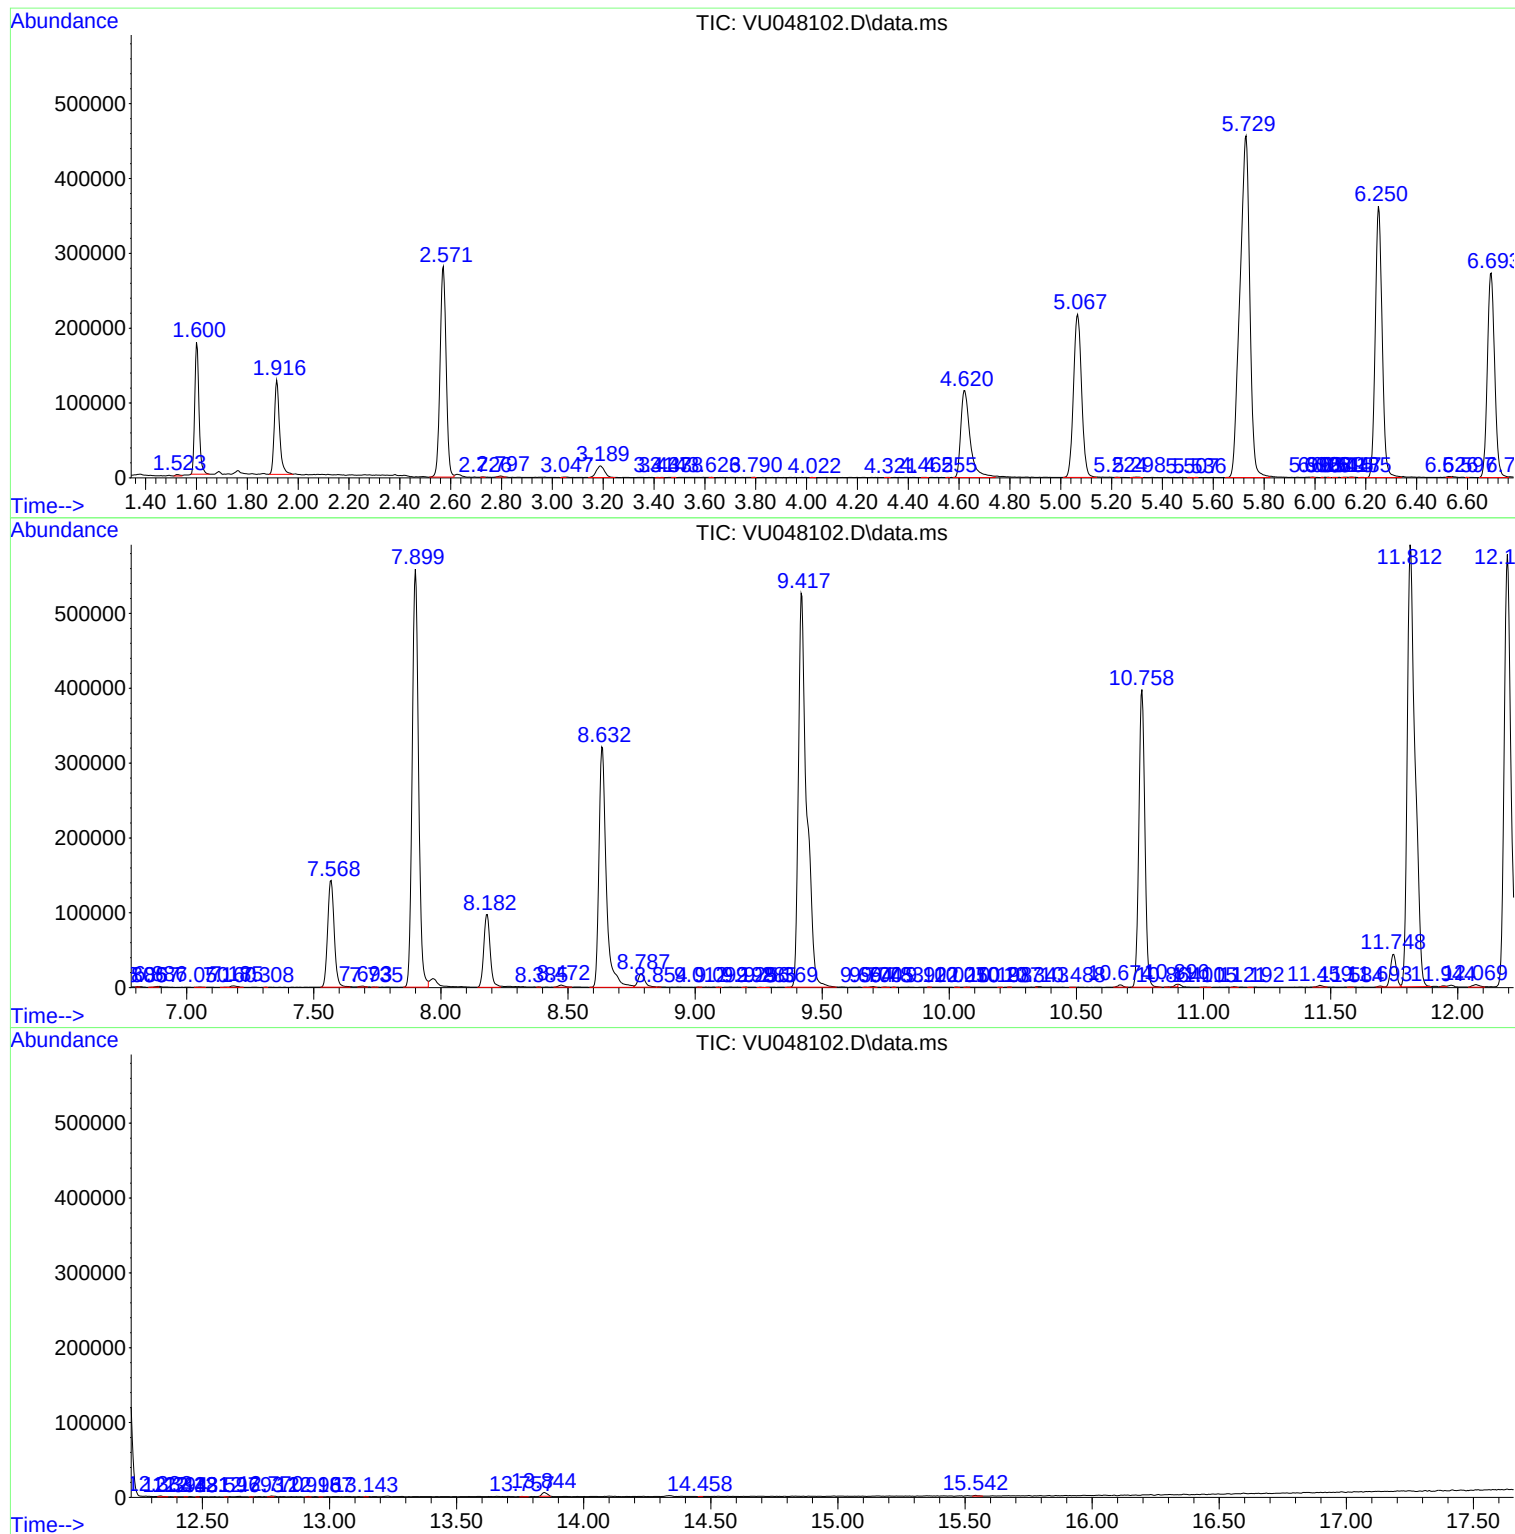

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048102.D
Acq On : 15 Apr 2022 14:58
Operator : SY/MD
Sample : N2386-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048102.D
Acq On : 15 Apr 2022 14:58
Operator : SY/MD
Sample : N2386-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------