

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048103.D
 Acq On : 15 Apr 2022 15:21
 Operator : SY/MD
 Sample : N2386-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	184030	253159	17.16%	2.324%
2	1.916	173	179	197	rVB	128117	182320	12.36%	1.673%
3	2.568	370	382	395	rBV	282689	466098	31.59%	4.278%
4	2.687	413	419	426	rVB6	1472	2376	0.16%	0.022%
5	2.797	446	453	468	rVB	5826	9975	0.68%	0.092%
6	2.858	468	472	473	rBV3	675	407	0.03%	0.004%
7	3.192	562	576	590	rBV	7098	16110	1.09%	0.148%
8	3.848	778	780	785	rVV3	550	452	0.03%	0.004%
9	3.880	786	790	791	rVV3	329	218	0.01%	0.002%
10	3.996	822	826	829	rBV2	281	239	0.02%	0.002%
11	4.115	861	863	867	rVB	414	293	0.02%	0.003%
12	4.138	867	870	872	rBV2	312	218	0.01%	0.002%
13	4.247	900	904	906	rBV2	328	283	0.02%	0.003%
14	4.279	910	914	921	rVV4	435	439	0.03%	0.004%
15	4.623	1008	1021	1051	rBV	116773	288826	19.58%	2.651%
16	5.067	1142	1159	1184	rVV	220276	480128	32.54%	4.407%
17	5.221	1203	1207	1210	rVB2	405	336	0.02%	0.003%
18	5.289	1222	1228	1234	rVV4	463	813	0.06%	0.007%
19	5.600	1323	1325	1333	rVB4	278	303	0.02%	0.003%
20	5.726	1343	1364	1394	rBV2	460181	1238870	83.97%	11.371%
21	5.864	1405	1407	1412	rVB3	414	264	0.02%	0.002%
22	5.964	1435	1438	1439	rBV	466	300	0.02%	0.003%
23	6.250	1512	1527	1550	rBV	450116	855210	57.97%	7.850%
24	6.488	1597	1601	1606	rVB3	209	223	0.02%	0.002%
25	6.523	1609	1612	1613	rBV	1172	655	0.04%	0.006%
26	6.591	1631	1633	1638	rVB3	345	224	0.02%	0.002%
27	6.694	1650	1665	1692	rBV	282367	553235	37.50%	5.078%
28	6.790	1692	1695	1697	rBV2	436	298	0.02%	0.003%
29	6.880	1720	1723	1724	rBV	482	281	0.02%	0.003%
30	6.954	1743	1746	1751	rBV2	227	253	0.02%	0.002%
31	7.182	1808	1817	1829	rVB6	2184	3577	0.24%	0.033%
32	7.247	1834	1837	1840	rVB	453	246	0.02%	0.002%
33	7.317	1850	1859	1860	rBV	315	357	0.02%	0.003%
34	7.407	1881	1887	1891	rBV3	350	350	0.02%	0.003%
35	7.443	1894	1898	1903	rVB2	302	305	0.02%	0.003%
36	7.472	1903	1907	1909	rBV	349	222	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048103.D
 Acq On : 15 Apr 2022 15:21
 Operator : SY/MD
 Sample : N2386-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.568	1916	1937	1954	rBV	143293	254392	17.24%	2.335%
38	7.655	1962	1964	1967	rVB3	441	270	0.02%	0.002%
39	7.690	1967	1975	1979	rBV6	1564	2185	0.15%	0.020%
40	7.784	1999	2004	2006	rVV3	347	361	0.02%	0.003%
41	7.803	2008	2010	2013	rVB2	409	257	0.02%	0.002%
42	7.899	2026	2040	2055	rBV	563206	973636	65.99%	8.937%
43	8.179	2116	2127	2145	rBV	100554	172642	11.70%	1.585%
44	8.472	2211	2218	2230	rVB2	2689	4024	0.27%	0.037%
45	8.523	2230	2234	2238	rBV4	383	352	0.02%	0.003%
46	8.633	2255	2268	2303	rBV	344038	644717	43.70%	5.918%
47	8.790	2312	2317	2333	rVB6	5590	8995	0.61%	0.083%
48	8.880	2344	2345	2349	rVB2	603	235	0.02%	0.002%
49	8.928	2357	2360	2367	rVB3	533	524	0.04%	0.005%
50	8.960	2367	2370	2375	rBV3	462	481	0.03%	0.004%
51	9.157	2427	2431	2433	rVV2	355	221	0.01%	0.002%
52	9.301	2471	2476	2479	rBV3	318	298	0.02%	0.003%
53	9.420	2499	2513	2516	rBV	704403	1095893	74.28%	10.059%
54	9.687	2592	2596	2598	rBV2	745	620	0.04%	0.006%
55	9.877	2650	2655	2658	rBV2	317	329	0.02%	0.003%
56	9.938	2670	2674	2679	rBV2	327	403	0.03%	0.004%
57	10.102	2721	2725	2729	rBV3	563	469	0.03%	0.004%
58	10.163	2739	2744	2747	rBV2	218	218	0.01%	0.002%
59	10.349	2798	2802	2809	rVB5	620	590	0.04%	0.005%
60	10.391	2813	2815	2818	rBV2	306	231	0.02%	0.002%
61	10.436	2826	2829	2833	rVB2	329	251	0.02%	0.002%
62	10.462	2833	2837	2838	rBV	339	222	0.02%	0.002%
63	10.671	2893	2902	2914	rVB5	3082	4747	0.32%	0.044%
64	10.758	2914	2929	2950	rBV	398864	645306	43.74%	5.923%
65	10.893	2959	2971	2982	rBV2	3913	7137	0.48%	0.066%
66	11.009	3002	3007	3008	rBV2	452	339	0.02%	0.003%
67	11.057	3015	3022	3025	rBV3	573	608	0.04%	0.006%
68	11.073	3025	3027	3031	rVB	579	349	0.02%	0.003%
69	11.112	3036	3039	3040	rBV	618	364	0.02%	0.003%
70	11.153	3049	3052	3056	rVB2	333	231	0.02%	0.002%
71	11.221	3068	3073	3078	rBV2	349	443	0.03%	0.004%
72	11.356	3109	3115	3117	rBV	371	361	0.02%	0.003%
73	11.459	3139	3147	3160	rVV8	2593	4966	0.34%	0.046%
74	11.578	3182	3184	3189	rVV3	407	320	0.02%	0.003%
75	11.642	3198	3204	3209	rVB3	301	375	0.03%	0.003%
76	11.697	3215	3221	3227	rBV5	1793	2323	0.16%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048103.D
 Acq On : 15 Apr 2022 15:21
 Operator : SY/MD
 Sample : N2386-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.745	3227	3236	3245	rBV	44364	68358	4.63%	0.627%
78	11.812	3245	3257	3280	rVB2	730516	1475365	100.00%	13.542%
79	11.931	3291	3294	3296	rBV3	1156	914	0.06%	0.008%
80	11.970	3303	3306	3318	rVB5	2974	4578	0.31%	0.042%
81	12.044	3326	3329	3330	rBV	405	236	0.02%	0.002%
82	12.066	3330	3336	3347	rVV5	5153	9214	0.62%	0.085%
83	12.121	3351	3353	3356	rVB3	623	390	0.03%	0.004%
84	12.195	3361	3376	3399	rVV2	587758	1128588	76.50%	10.359%
85	12.275	3399	3401	3405	rVB2	700	437	0.03%	0.004%
86	12.330	3415	3418	3425	rVB3	1504	1552	0.11%	0.014%
87	12.359	3425	3427	3430	rBV4	342	292	0.02%	0.003%
88	12.404	3438	3441	3448	rVB3	764	792	0.05%	0.007%
89	12.539	3480	3483	3485	rBV2	455	322	0.02%	0.003%
90	12.571	3490	3493	3496	rBV2	418	277	0.02%	0.003%
91	12.636	3511	3513	3515	rBV	525	321	0.02%	0.003%
92	12.722	3537	3540	3543	rBV3	328	240	0.02%	0.002%
93	12.774	3553	3556	3564	rBV3	679	931	0.06%	0.009%
94	12.890	3590	3592	3594	rBV2	495	309	0.02%	0.003%
95	13.060	3642	3645	3648	rBV3	331	263	0.02%	0.002%
96	13.150	3669	3673	3678	rVB3	591	543	0.04%	0.005%
97	13.845	3880	3889	3900	rVB5	5478	9179	0.62%	0.084%
98	13.896	3900	3905	3910	rBV3	477	634	0.04%	0.006%
99	14.330	4036	4040	4049	rVV4	1232	1699	0.12%	0.016%
100	15.195	4306	4309	4315	rBV4	654	728	0.05%	0.007%




Sum of corrected areas: 10894710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048103.D
Acq On : 15 Apr 2022 15:21
Operator : SY/MD
Sample : N2386-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

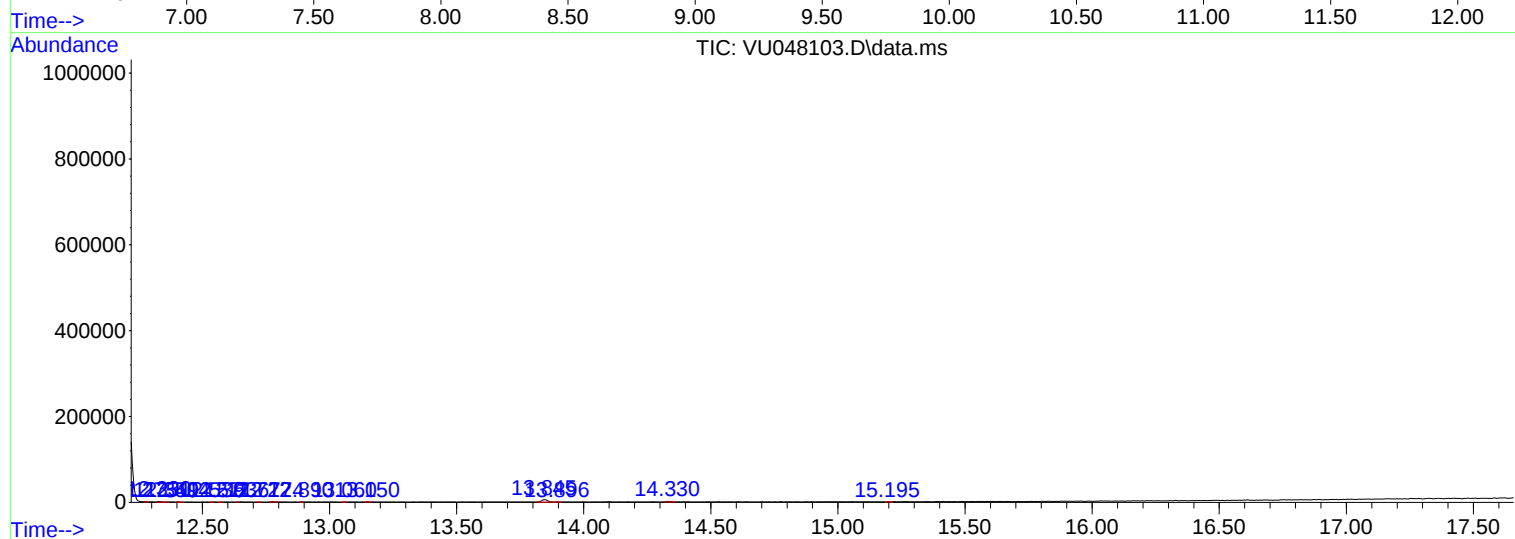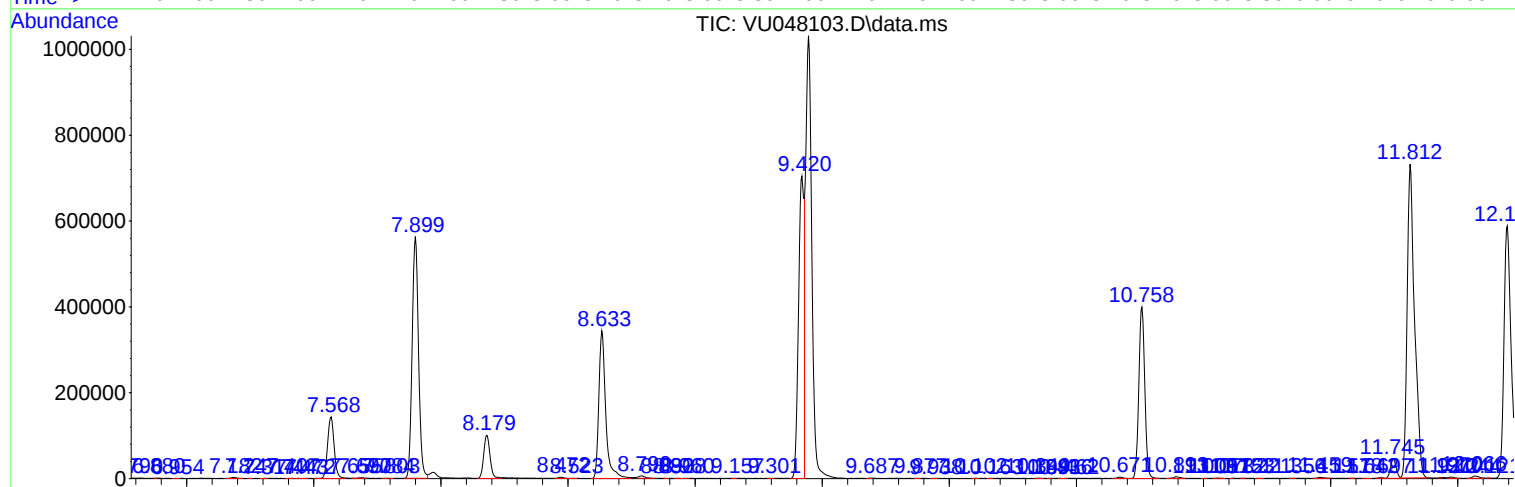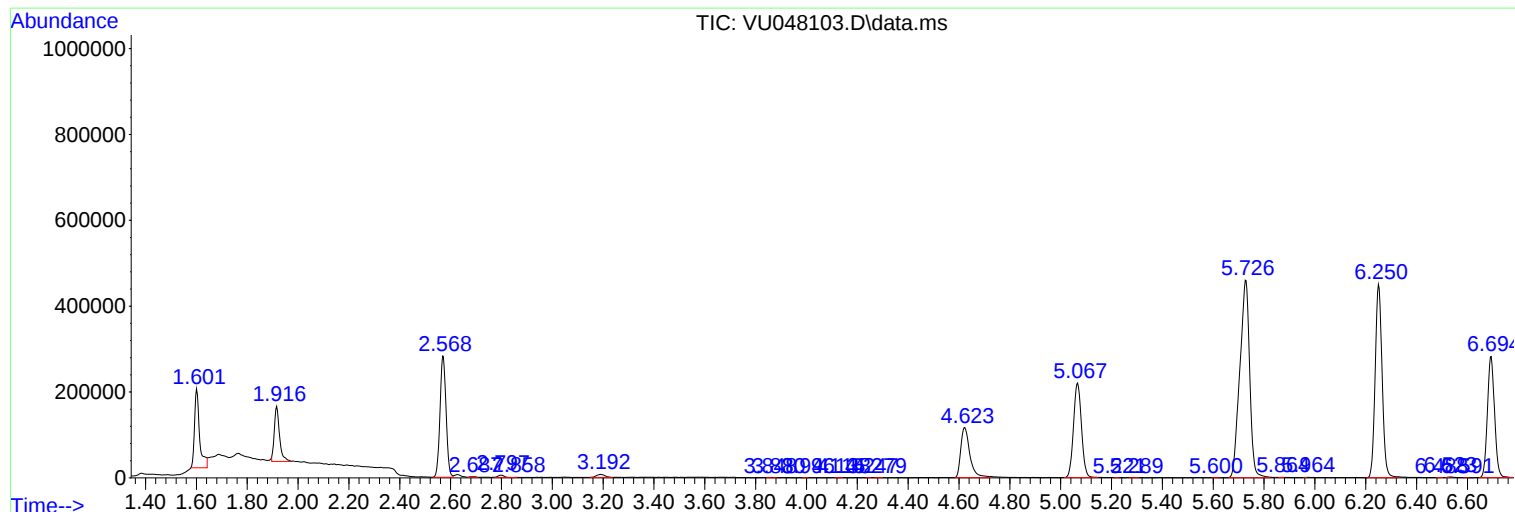

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048103.D
Acq On : 15 Apr 2022 15:21
Operator : SY/MD
Sample : N2386-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048103.D
Acq On : 15 Apr 2022 15:21
Operator : SY/MD
Sample : N2386-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc