

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048104.D
 Acq On : 15 Apr 2022 16:27
 Operator : SY/MD
 Sample : VIBLK061
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rBV	160904	191582	15.91%	1.903%
2	1.916	171	179	206	rVB	122750	178977	14.86%	1.777%
3	2.568	370	382	400	rBV	273907	448041	37.20%	4.449%
4	2.735	427	434	442	rVB3	562	979	0.08%	0.010%
5	2.797	449	453	455	rBV3	300	184	0.02%	0.002%
6	2.954	497	502	504	rBV3	487	426	0.04%	0.004%
7	2.980	508	510	515	rVB2	352	226	0.02%	0.002%
8	3.051	523	532	543	rBV3	4132	7770	0.65%	0.077%
9	3.160	561	566	568	rBV3	287	216	0.02%	0.002%
10	3.192	575	576	582	rVB2	358	237	0.02%	0.002%
11	3.231	586	588	593	rBV2	195	212	0.02%	0.002%
12	3.305	607	611	613	rBV2	552	410	0.03%	0.004%
13	3.317	613	615	619	rVV	310	225	0.02%	0.002%
14	3.446	649	655	659	rBV3	410	406	0.03%	0.004%
15	3.546	684	686	689	rBV2	292	208	0.02%	0.002%
16	3.562	689	691	696	rVB	272	242	0.02%	0.002%
17	3.629	707	712	713	rBV	259	202	0.02%	0.002%
18	3.642	713	716	721	rVV2	279	252	0.02%	0.003%
19	3.726	739	742	747	rBV3	315	290	0.02%	0.003%
20	3.832	771	775	779	rBV3	256	291	0.02%	0.003%
21	3.854	779	782	788	rVV3	271	299	0.02%	0.003%
22	3.935	804	807	812	rBV2	300	318	0.03%	0.003%
23	4.057	842	845	847	rVB	322	191	0.02%	0.002%
24	4.150	870	874	876	rVB2	363	280	0.02%	0.003%
25	4.224	890	897	899	rBV3	506	530	0.04%	0.005%
26	4.288	914	917	923	rBV2	398	436	0.04%	0.004%
27	4.375	941	944	948	rVB	302	195	0.02%	0.002%
28	4.427	956	960	964	rBV2	252	319	0.03%	0.003%
29	4.546	991	997	1001	rBV2	211	272	0.02%	0.003%
30	4.626	1009	1022	1058	rBV	109876	277599	23.05%	2.757%
31	4.858	1090	1094	1100	rBV2	269	296	0.02%	0.003%
32	4.960	1122	1126	1129	rVB2	217	186	0.02%	0.002%
33	5.063	1140	1158	1181	rBV	213089	472954	39.27%	4.697%
34	5.208	1199	1203	1209	rVB3	514	583	0.05%	0.006%
35	5.237	1209	1212	1216	rBV2	253	219	0.02%	0.002%
36	5.269	1217	1222	1223	rBV2	267	205	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048104.D
 Acq On : 15 Apr 2022 16:27
 Operator : SY/MD
 Sample : VIBLK061
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.333	1239	1242	1247	rBV2	330	300	0.02%	0.003%
38	5.391	1254	1260	1263	rVB2	412	485	0.04%	0.005%
39	5.536	1300	1305	1309	rBV2	298	284	0.02%	0.003%
40	5.726	1340	1364	1391	rBV2	450284	1204466	100.00%	11.961%
41	6.041	1459	1462	1464	rBV2	402	208	0.02%	0.002%
42	6.250	1512	1527	1551	rBV	456689	867951	72.06%	8.620%
43	6.539	1609	1617	1625	rVB4	1581	2666	0.22%	0.026%
44	6.690	1650	1664	1686	rBV	273542	536621	44.55%	5.329%
45	6.806	1697	1700	1712	rVB5	769	850	0.07%	0.008%
46	7.038	1769	1772	1774	rBV	352	249	0.02%	0.002%
47	7.185	1809	1818	1827	rVV5	2001	3433	0.29%	0.034%
48	7.340	1861	1866	1869	rBV2	253	305	0.03%	0.003%
49	7.478	1899	1909	1915	rBV2	412	613	0.05%	0.006%
50	7.565	1924	1936	1958	rBV	139662	249602	20.72%	2.479%
51	7.684	1969	1973	1984	rVB5	1423	2086	0.17%	0.021%
52	7.899	2021	2040	2056	rBV	542887	950776	78.94%	9.442%
53	8.179	2114	2127	2143	rBV	98741	168927	14.03%	1.678%
54	8.439	2205	2208	2213	rVB3	255	211	0.02%	0.002%
55	8.507	2227	2229	2233	rVV3	445	255	0.02%	0.003%
56	8.636	2256	2269	2300	rBV	341480	642425	53.34%	6.380%
57	9.076	2403	2406	2411	rVB2	415	321	0.03%	0.003%
58	9.102	2411	2414	2418	rBV	263	239	0.02%	0.002%
59	9.295	2471	2474	2475	rBV	359	185	0.02%	0.002%
60	9.330	2483	2485	2489	rBV2	380	269	0.02%	0.003%
61	9.417	2498	2512	2554	rBV	654527	1126646	93.54%	11.189%
62	9.571	2559	2560	2562	rBV	480	225	0.02%	0.002%
63	9.587	2562	2565	2569	rVB3	531	322	0.03%	0.003%
64	9.642	2578	2582	2584	rBV2	212	200	0.02%	0.002%
65	9.690	2587	2597	2608	rBV3	532	1024	0.09%	0.010%
66	9.861	2643	2650	2653	rBV2	181	261	0.02%	0.003%
67	9.883	2655	2657	2661	rVB2	332	233	0.02%	0.002%
68	10.066	2711	2714	2719	rVB2	281	257	0.02%	0.003%
69	10.304	2784	2788	2792	rBV	261	252	0.02%	0.003%
70	10.472	2837	2840	2844	rVB2	356	213	0.02%	0.002%
71	10.526	2854	2857	2861	rVV2	324	204	0.02%	0.002%
72	10.562	2865	2868	2874	rVB2	291	268	0.02%	0.003%
73	10.671	2893	2902	2911	rVB4	2647	4079	0.34%	0.041%
74	10.758	2915	2929	2949	rVV	392100	633866	52.63%	6.295%
75	10.873	2960	2965	2967	rBV2	458	383	0.03%	0.004%
76	10.922	2977	2980	2987	rVV2	468	402	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048104.D
 Acq On : 15 Apr 2022 16:27
 Operator : SY/MD
 Sample : VIBLK061
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.086	3027	3031	3034	rVB3	327	280	0.02%	0.003%
78	11.118	3034	3041	3044	rBV4	591	575	0.05%	0.006%
79	11.208	3065	3069	3071	rBV2	401	283	0.02%	0.003%
80	11.285	3091	3093	3099	rBV2	245	189	0.02%	0.002%
81	11.381	3118	3123	3126	rVB2	247	222	0.02%	0.002%
82	11.459	3139	3147	3156	rVB3	1006	1775	0.15%	0.018%
83	11.581	3179	3185	3186	rBV3	391	359	0.03%	0.004%
84	11.639	3198	3203	3208	rBV2	287	353	0.03%	0.004%
85	11.700	3218	3222	3226	rVB4	966	837	0.07%	0.008%
86	11.751	3232	3238	3243	rVB4	743	905	0.08%	0.009%
87	11.812	3243	3257	3281	rBV	723475	1152115	95.65%	11.442%
88	11.973	3304	3307	3313	rVB5	2045	2018	0.17%	0.020%
89	12.086	3338	3342	3345	rVB3	385	317	0.03%	0.003%
90	12.115	3349	3351	3357	rVB3	285	222	0.02%	0.002%
91	12.192	3362	3375	3394	rBV	547406	913704	75.86%	9.074%
92	12.333	3413	3419	3423	rVB5	1264	1413	0.12%	0.014%
93	12.365	3427	3429	3435	rVB4	427	331	0.03%	0.003%
94	12.397	3435	3439	3441	rBV2	355	300	0.02%	0.003%
95	12.606	3500	3504	3507	rVB2	253	207	0.02%	0.002%
96	12.642	3512	3515	3519	rVB3	547	500	0.04%	0.005%
97	12.793	3559	3562	3564	rBV	265	185	0.02%	0.002%
98	12.970	3614	3617	3620	rBV3	326	251	0.02%	0.002%
99	13.848	3884	3890	3897	rBV3	2663	3090	0.26%	0.031%
100	15.436	4381	4384	4385	rBV2	510	325	0.03%	0.003%




Sum of corrected areas: 10069576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048104.D
Acq On : 15 Apr 2022 16:27
Operator : SY/MD
Sample : VIBLK061
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

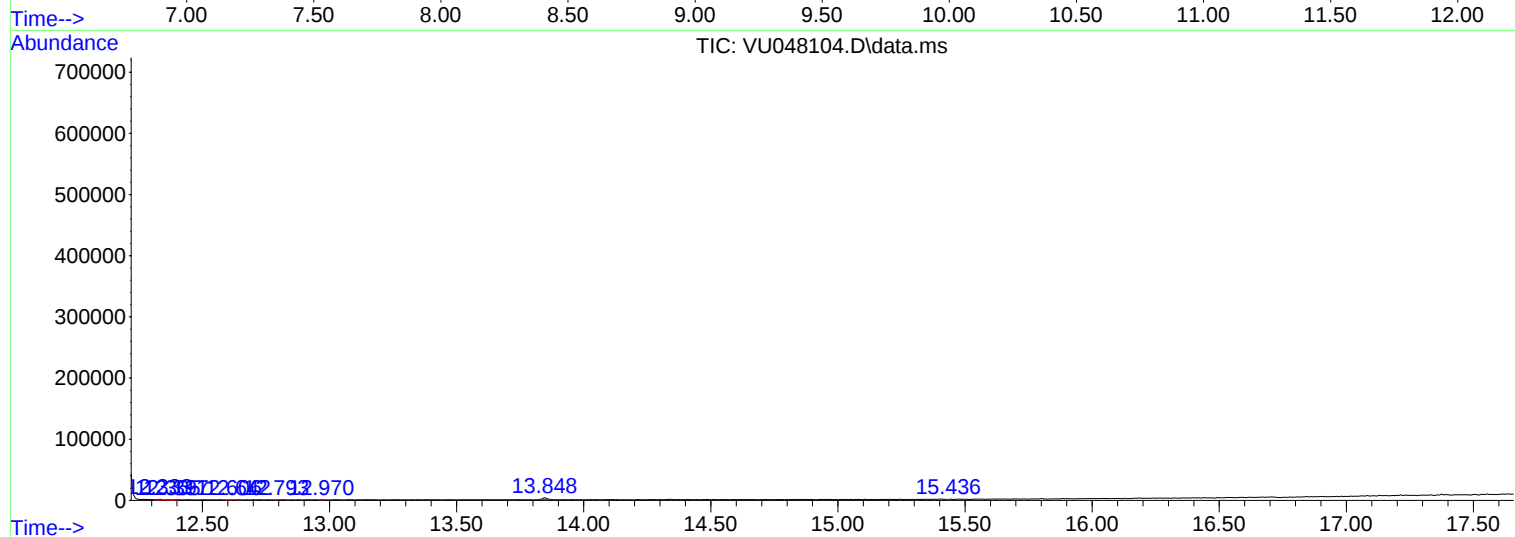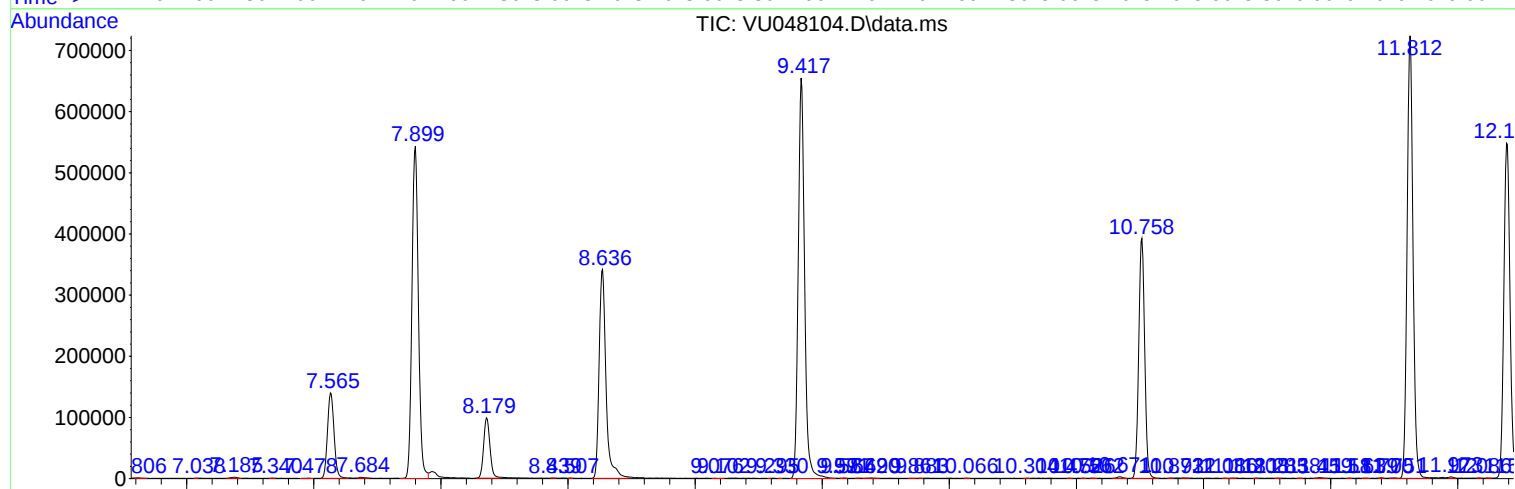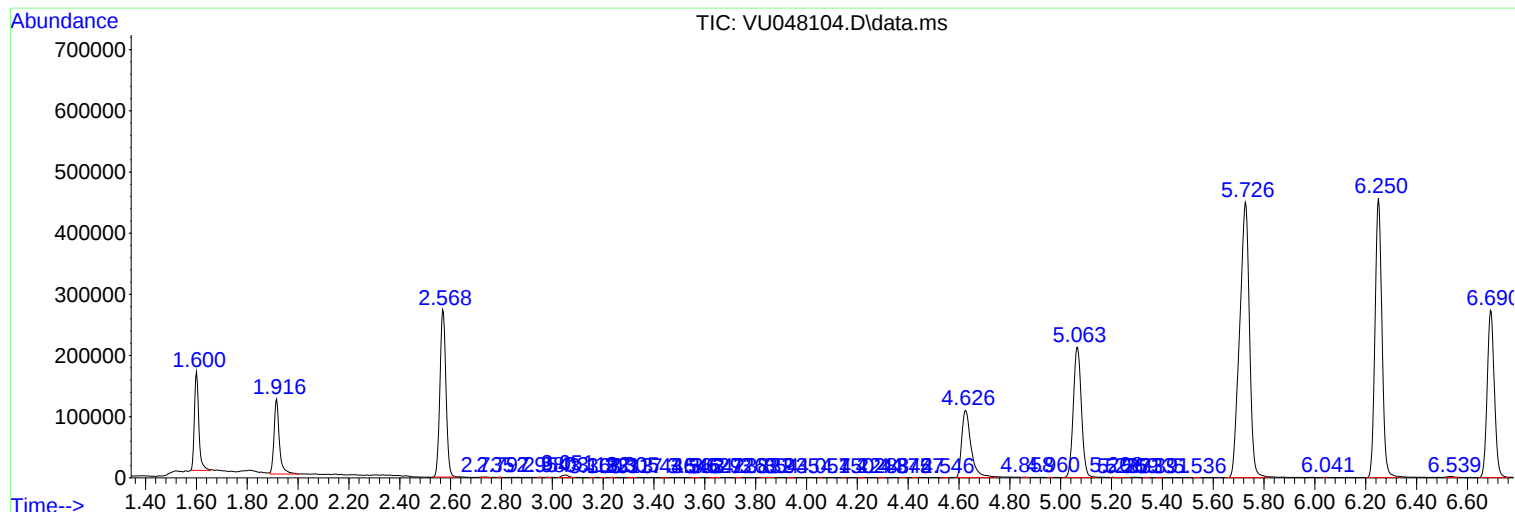

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048104.D
Acq On : 15 Apr 2022 16:27
Operator : SY/MD
Sample : VIBLK061
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
Data File : VU048104.D
Acq On : 15 Apr 2022 16:27
Operator : SY/MD
Sample : VIBLK061
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK061

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
