


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041522\
 Data File : VU048093.D
 Acq On : 15 Apr 2022 09:36
 Operator : SY/MD
 Sample : BFB065
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB065

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Wed Apr 20 02:08:53 2022

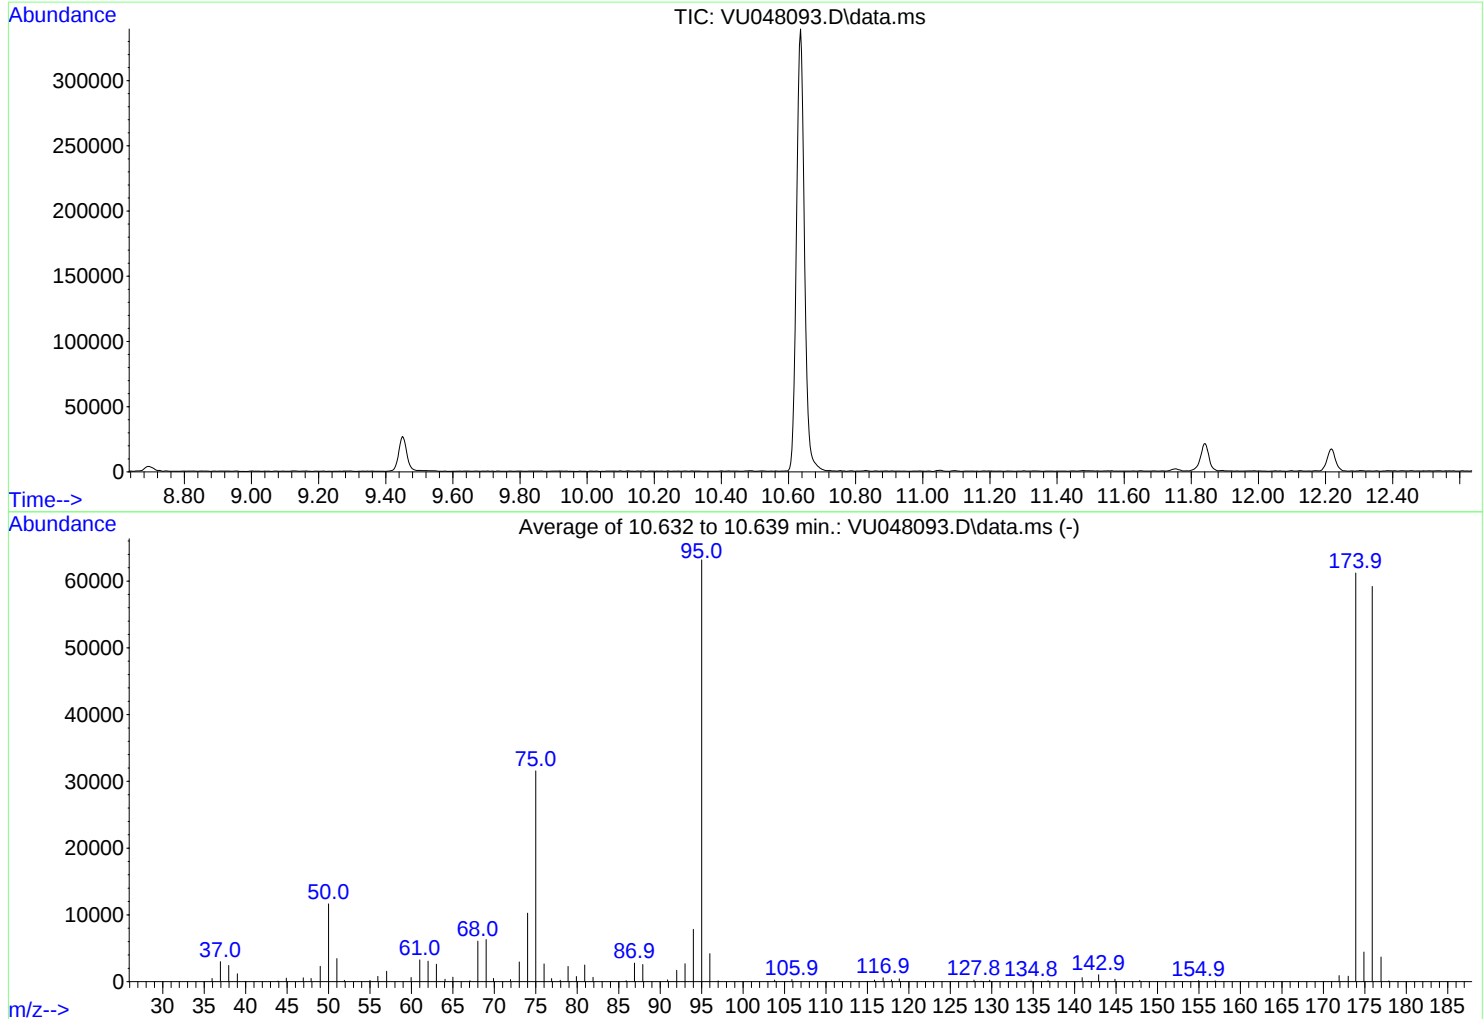

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	11657	PASS
75	95	30	80	50.0	31563	PASS
95	95	100	100	100.0	63184	PASS
96	95	5	9	6.6	4194	PASS
173	174	0.00	2	1.3	821	PASS
174	95	50	120	96.9	61219	PASS
175	174	5	9	7.2	4430	PASS
176	174	95	101	96.7	59195	PASS
177	176	5	9	6.2	3687	PASS

m/z	Abundance
40.00	174.0
44.00	525.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	505.0
37.00	2941.0
38.00	2529.0
39.00	1246.0
39.90	232.0
43.90	646.0
44.90	552.0
47.00	614.0
47.90	502.0
49.00	2381.0
50.00	11591.0
51.00	3554.0
51.90	174.0
55.00	220.0
55.90	772.0
57.00	1542.0
60.00	590.0
61.00	3351.0
62.00	3067.0
63.00	2683.0
64.00	354.0
65.00	683.0
67.10	153.0
68.00	6168.0
69.00	6509.0
69.90	469.0
72.00	330.0
73.00	2968.0
74.00	10277.0
75.00	32040.0
76.00	2738.0
76.90	459.0
78.00	226.0
78.90	2216.0
79.90	798.0
80.90	2445.0
81.90	583.0
85.90	143.0
86.90	2756.0
87.90	2508.0
90.90	296.0
92.00	1734.0
93.00	2573.0
94.00	7698.0
95.00	62832.0
96.00	4311.0
97.10	166.0
103.80	249.0
105.90	318.0
115.80	242.0
116.90	634.0
117.90	241.0
118.80	448.0
127.90	218.0
128.70	131.0
129.70	227.0
134.80	125.0
136.80	151.0
140.90	562.0
141.70	122.0
142.90	1056.0
144.90	370.0
147.80	196.0
154.90	140.0
156.90	115.0
171.90	900.0
173.00	796.0
173.90	59824.0
174.90	4459.0
175.90	57400.0
176.90	3693.0
177.90	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	486.0
37.00	3095.0
38.00	2480.0
39.00	1212.0
39.90	217.0
43.90	627.0
44.90	559.0
46.90	576.0
47.90	513.0
49.00	2353.0
50.00	12031.0
51.00	3519.0
51.90	192.0
55.00	212.0
55.90	807.0
57.00	1573.0
60.00	626.0
61.00	3397.0
62.00	3145.0
63.00	2698.0
64.00	382.0
65.00	701.0
67.10	161.0
68.00	6220.0
69.00	6503.0
69.90	497.0
72.00	310.0
73.00	3038.0
74.00	10570.0
75.00	32448.0
76.00	2689.0
76.90	466.0
78.00	224.0
78.90	2335.0
79.90	788.0
80.90	2603.0
81.90	672.0
85.90	160.0
86.90	2894.0
87.90	2614.0
90.90	256.0
92.00	1735.0
93.00	2760.0
94.00	8220.0
95.00	65152.0
96.00	4347.0
97.00	121.0
103.80	242.0
105.90	316.0
115.00	119.0
115.90	257.0
116.90	590.0
117.90	297.0
118.90	455.0
127.90	239.0
128.70	130.0
129.80	232.0
134.70	147.0
136.80	159.0
140.90	620.0
142.90	1076.0
144.80	384.0
147.80	227.0
155.00	165.0
157.00	136.0
171.90	904.0
173.00	865.0
173.90	63088.0
174.90	4543.0
175.90	61288.0
177.00	3774.0
177.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
35.90	449.0
36.90	2956.0
37.90	2270.0
39.00	1102.0
40.00	198.0
43.80	588.0
44.90	454.0
47.00	528.0
47.90	453.0
49.00	2205.0
50.00	11348.0
51.00	3296.0
51.90	188.0
55.00	167.0
56.00	810.0
57.00	1529.0
59.90	626.0
61.00	3032.0
62.00	3032.0
63.00	2472.0
64.10	389.0
65.00	649.0
67.00	149.0
68.00	5806.0
69.00	5919.0
69.90	501.0
71.90	317.0
73.00	2840.0
74.00	9923.0
75.00	30200.0
76.00	2539.0
76.90	429.0
77.90	226.0
78.90	2292.0
79.90	740.0
80.90	2465.0
81.90	654.0
85.90	151.0
86.90	2665.0
87.90	2551.0
90.90	248.0
92.00	1650.0
93.00	2713.0
94.00	7597.0
95.00	61568.0
96.00	3923.0
96.90	108.0
103.80	241.0
105.90	281.0
115.90	226.0
116.90	501.0
117.90	291.0
118.90	412.0
127.80	238.0
128.90	113.0
129.80	224.0
134.70	131.0
136.80	132.0
140.90	627.0
142.90	963.0
144.90	366.0
147.90	194.0
155.00	175.0
156.90	132.0
171.90	911.0
173.00	801.0
173.90	60744.0
174.90	4288.0
175.90	58896.0
176.90	3593.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065