

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041524\
 Data File : VU058698.D
 Acq On : 15 Apr 2024 18:29
 Operator : MD/SY
 Sample : P2055-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COBM7

Quant Time: Apr 16 00:42:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Apr 16 00:38:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	65683	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	66354	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	27776	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	15189	3.493	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.800%
7) Chloroethane-d5	1.904	69	17366	4.595	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.000%
11) 1,1-Dichloroethene-d2	2.560	65	7331	3.725	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.400%
20) 2-Butanone-d5	4.615	46	56878	62.065	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.120%
24) Chloroform-d	5.052	84	42452	4.890	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.692	65	22100	5.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.200%
32) Benzene-d6	5.717	84	75586	4.231	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
36) 1,2-Dichloropropane-d6	6.682	67	27361	4.884	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.894	98	55974	3.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.600%
43) trans-1,3-Dichloroprop...	8.177	79	6786	3.902	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%
46) 2-Hexanone-d5	8.630	63	37091	51.711	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.420%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	19318	4.884	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	19861	4.245	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.000%
Target Compounds						Qvalue
16) Methylene chloride	3.036	84	971	0.157	ug/L	88
47) Tetrachloroethene	8.547	164	37089	8.345	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041524\
Data File : VU058698.D
Acq On : 15 Apr 2024 18:29
Operator : MD/SY
Sample : P2055-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BM7

Quant Time: Apr 16 00:42:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Apr 16 00:38:11 2024
Response via : Initial Calibration




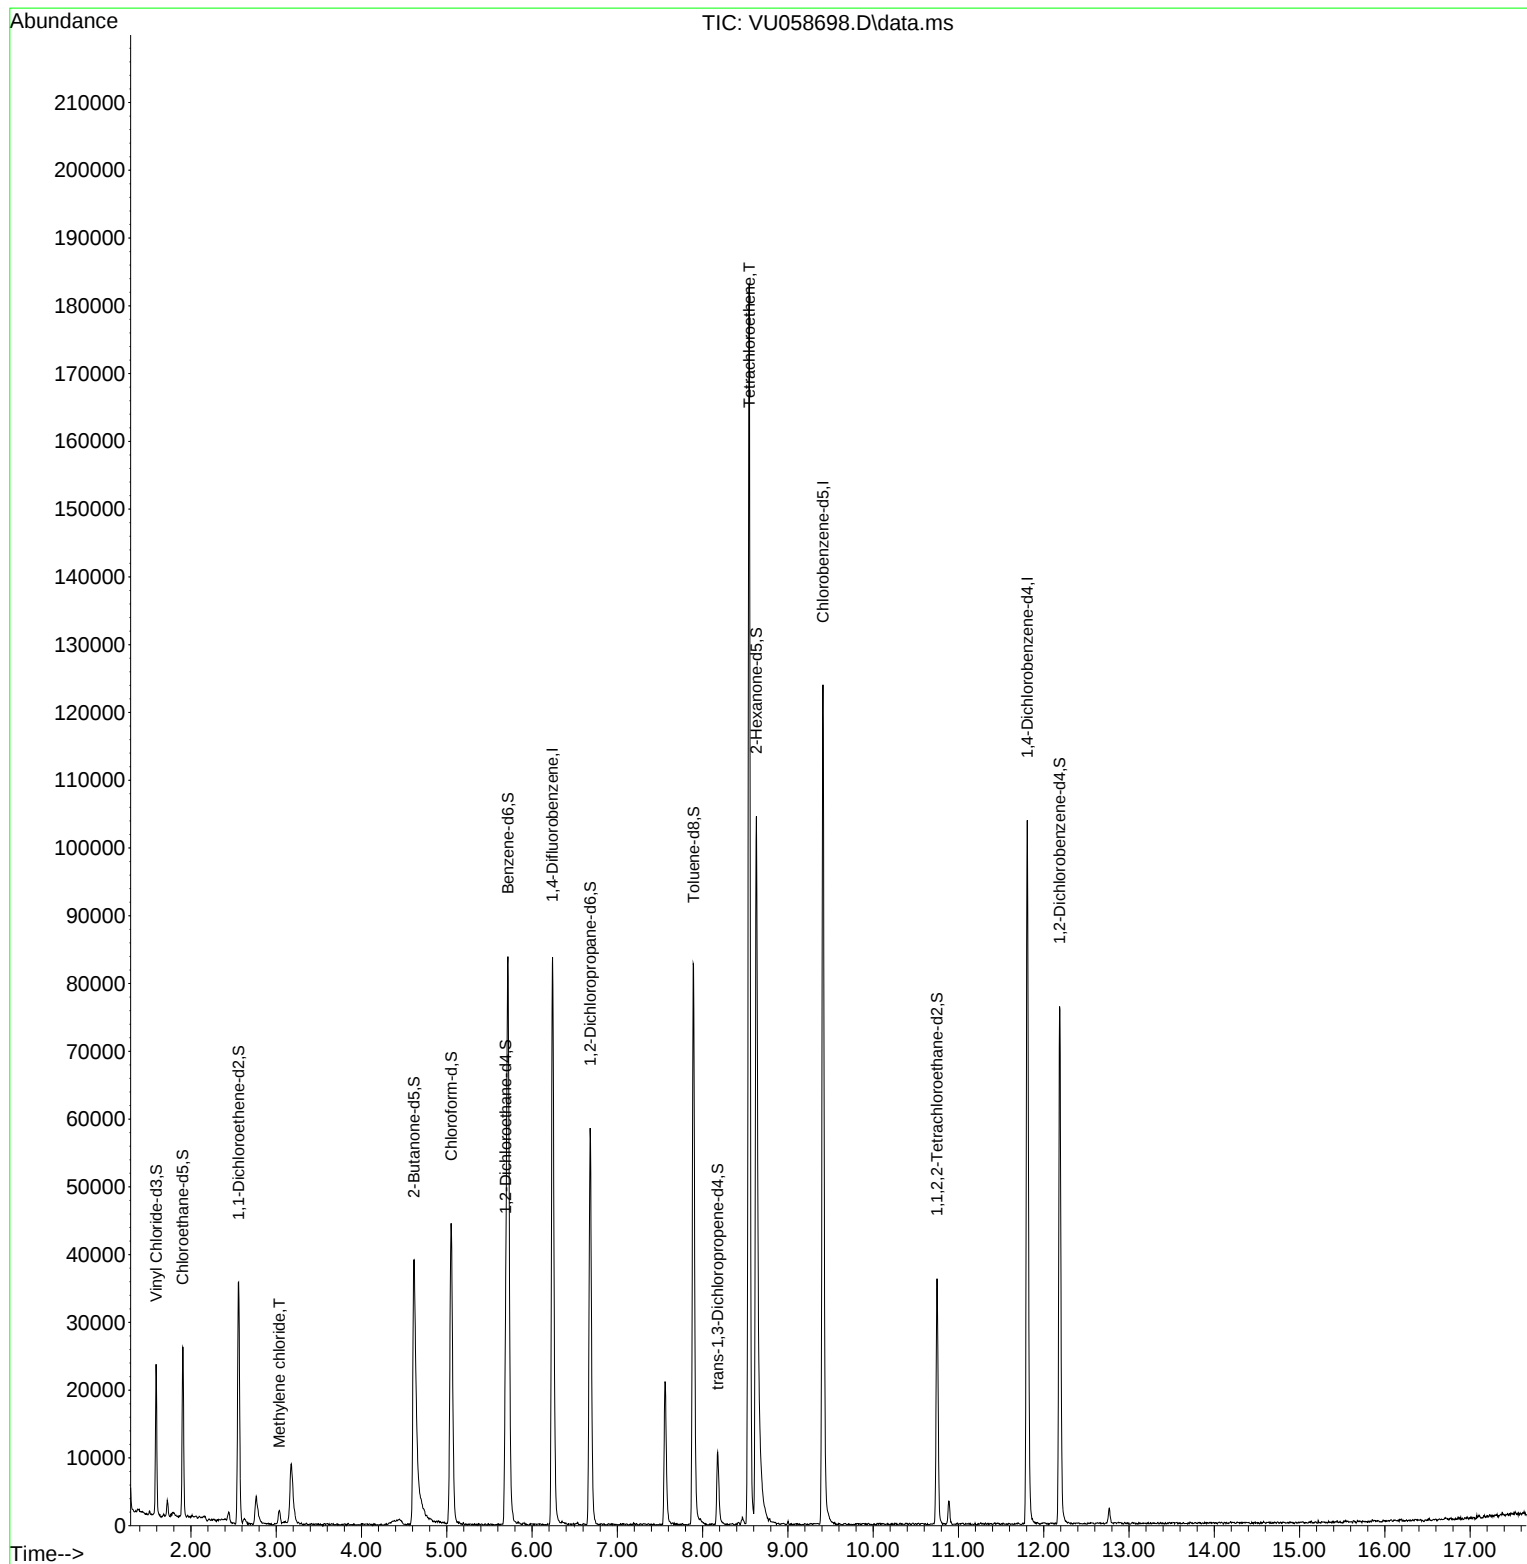


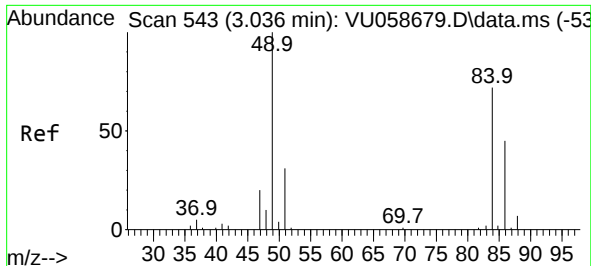

#16
Methylene chloride
Concen: 0.157 ug/L
RT: 3.036 min Scan# 543
Delta R.T. -0.000 min
Lab File: VU058698.D
Acq: 15 Apr 2024 18:29

Instrument :
MSVOA_U
ClientSampleId :
C0BM7

Tgt Ion: 84 Resp: 971
Ion Ratio Lower Upper
84 100
86 56.5 44.3 82.3
49 120.4 96.0 178.2

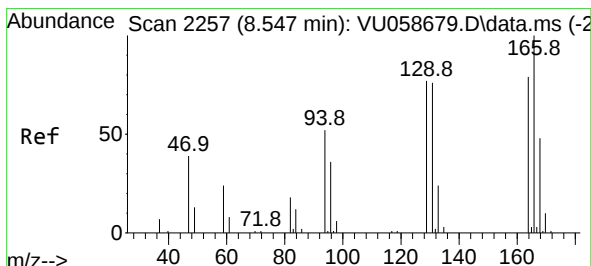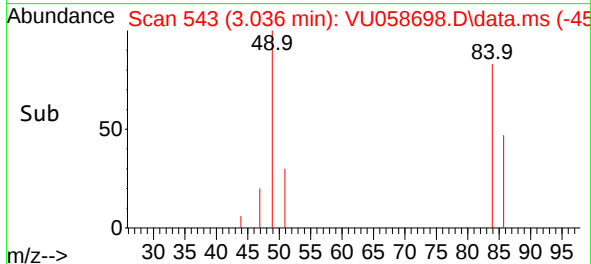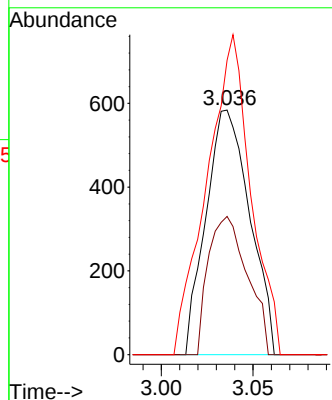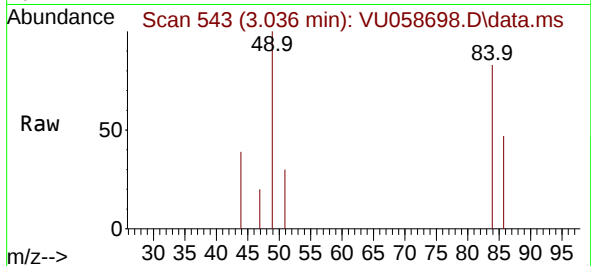

#47
Tetrachloroethene
Concen: 8.345 ug/L
RT: 8.547 min Scan# 2257
Delta R.T. -0.000 min
Lab File: VU058698.D
Acq: 15 Apr 2024 18:29

Tgt Ion: 164 Resp: 37089
Ion Ratio Lower Upper
164 100
129 101.3 67.3 125.1
131 97.7 65.5 121.6
166 129.0 89.5 166.1

