


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041524\
Data File : VU058678.D
Acq On : 15 Apr 2024 08:45
Operator : MD/SY
Sample : BFB143
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB143

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 16 00:38:11 2024

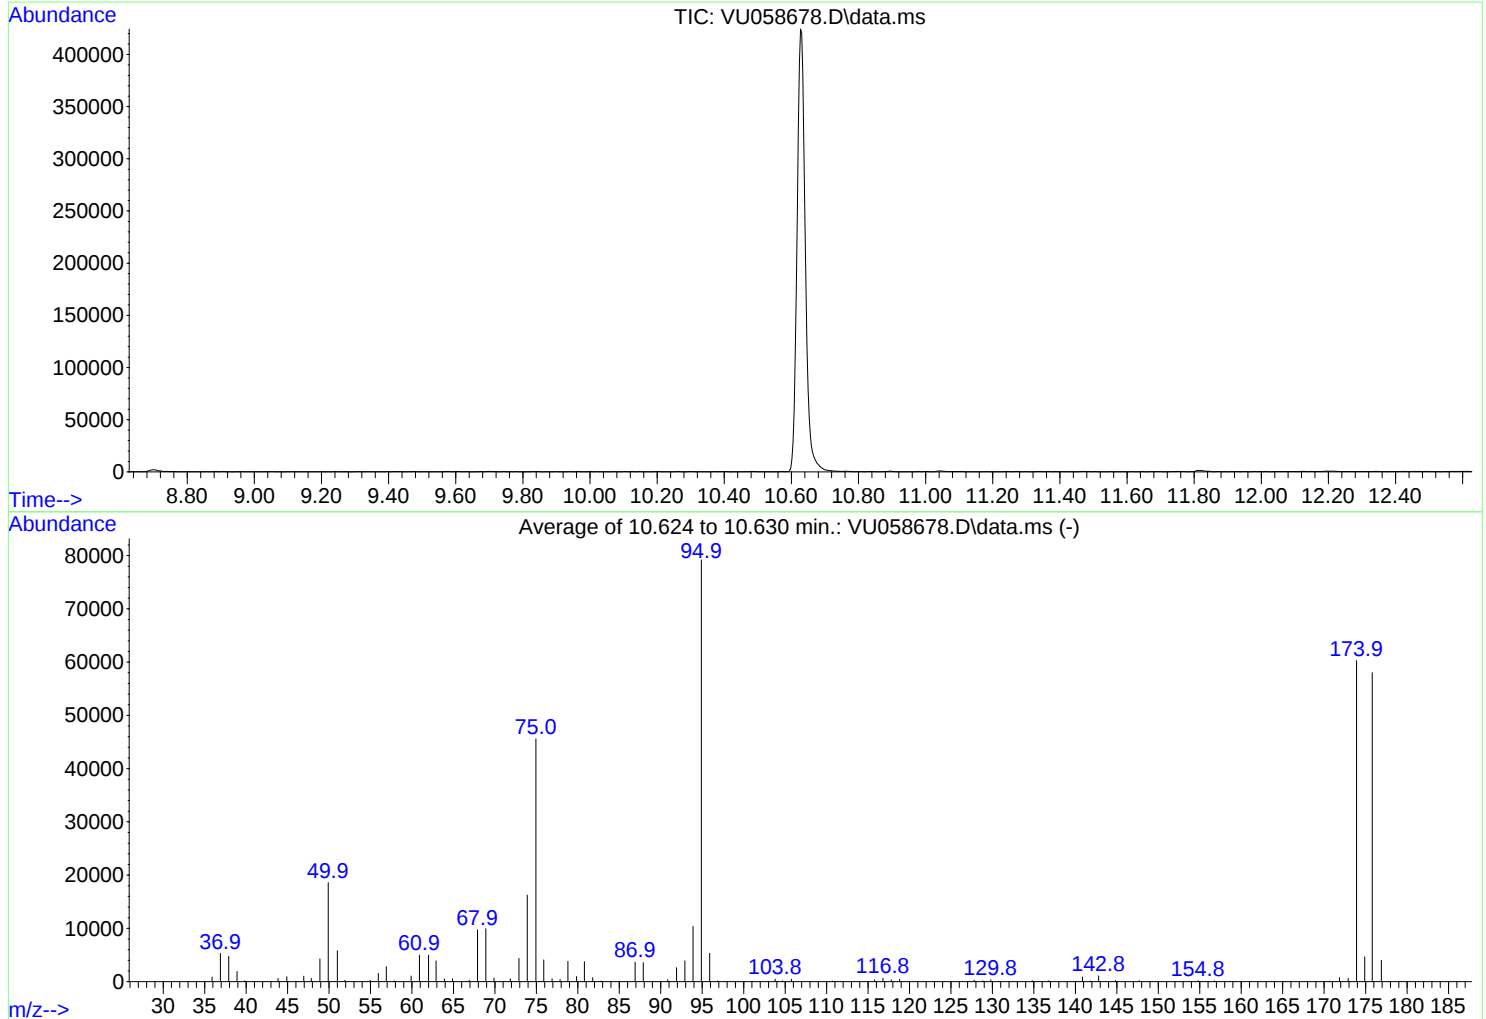

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	18603	PASS
75	95	30	80	57.5	45571	PASS
95	95	100	100	100.0	79203	PASS
96	95	5	9	6.7	5328	PASS
173	174	0.00	2	1.0	616	PASS
174	95	50	120	76.1	60261	PASS
175	174	5	9	7.7	4655	PASS
176	174	95	101	96.3	58003	PASS
177	176	5	9	6.9	4009	PASS

m/z	Abundance
43.80	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
35.90	887.0
36.90	5143.0
37.90	4563.0
38.90	1805.0
39.80	192.0
43.90	719.0
44.90	844.0
46.00	133.0
46.90	1044.0
47.80	574.0
48.90	4010.0
49.90	18080.0
51.00	5653.0
51.90	228.0
55.00	277.0
55.90	1574.0
56.90	2817.0
57.90	174.0
59.90	1018.0
60.90	4710.0
62.00	4645.0
62.90	3855.0
63.90	484.0
64.90	561.0
66.90	273.0
67.90	9412.0
68.90	9432.0
69.90	633.0
71.80	508.0
72.90	4174.0
73.90	15476.0
75.00	43832.0
75.90	3930.0
76.90	534.0
77.80	367.0
78.80	3747.0
79.80	988.0
80.80	3609.0
81.80	761.0
82.80	104.0
86.90	3455.0
87.90	3618.0
90.80	355.0
91.90	2493.0
92.90	3737.0
93.90	9968.0
94.90	75072.0
95.90	5303.0
96.90	147.0
103.80	444.0
104.70	144.0
105.80	393.0
110.70	119.0
115.80	311.0
116.80	605.0
117.80	305.0
118.80	409.0
127.80	230.0
128.80	135.0
129.80	368.0
130.80	121.0
134.80	173.0
136.80	159.0
140.80	852.0
141.80	123.0
142.80	1083.0
144.80	213.0
147.70	156.0
154.70	170.0
156.80	156.0
158.70	110.0
171.90	710.0
172.90	898.0
173.90	56320.0
174.90	4385.0
175.80	53616.0
176.90	3735.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
35.90	893.0
36.90	5441.0
37.90	4925.0
38.90	1956.0
39.90	188.0
43.90	780.0
44.90	957.0
46.00	129.0
46.90	1037.0
47.90	607.0
48.90	4435.0
49.90	19168.0
51.00	5947.0
51.90	235.0
55.00	287.0
55.90	1603.0
56.90	2895.0
57.90	159.0
59.90	1084.0
60.90	5205.0
62.00	5137.0
62.90	4042.0
63.90	529.0
64.90	570.0
66.90	268.0
67.90	10083.0
68.90	10263.0
69.90	671.0
71.80	537.0
72.90	4548.0
73.90	16752.0
74.90	46888.0
75.90	4240.0
76.90	568.0
77.80	386.0
78.80	3929.0
79.90	1007.0
80.80	3854.0
81.80	774.0
82.80	122.0
86.90	3815.0
87.90	3674.0
90.80	351.0
91.90	2681.0
92.90	4031.0
93.90	10709.0
94.90	81456.0
95.90	5496.0
96.90	138.0
103.80	488.0
104.70	173.0
105.70	475.0
110.70	145.0
115.80	340.0
116.80	664.0
117.80	329.0
118.80	425.0
127.80	286.0
128.90	151.0
129.80	337.0
130.80	100.0
134.80	184.0
136.80	189.0
140.80	886.0
141.80	131.0
142.80	1136.0
144.80	216.0
147.70	176.0
154.80	174.0
156.80	159.0
158.70	103.0
170.70	122.0
171.80	787.0
173.90	61976.0
174.90	4743.0
175.80	59800.0
176.90	4201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143

m/z	Abundance
35.90	860.0
36.90	5307.0
37.90	4771.0
38.90	1928.0
39.90	163.0
43.90	777.0
44.90	998.0
47.00	996.0
47.90	621.0
48.90	4383.0
49.90	18560.0
51.00	5829.0
51.90	222.0
54.90	287.0
56.00	1514.0
56.90	2771.0
57.80	149.0
59.90	1027.0
60.90	5069.0
62.00	5084.0
62.90	3867.0
63.90	500.0
64.90	518.0
66.90	243.0
67.90	9721.0
68.90	10111.0
69.90	660.0
71.90	550.0
72.90	4402.0
73.90	16512.0
74.90	45992.0
75.90	4113.0
76.90	537.0
77.90	402.0
78.80	3782.0
79.90	927.0
80.80	3776.0
81.80	728.0
82.80	112.0
86.90	3715.0
87.90	3451.0
90.90	354.0
91.90	2705.0
92.90	3976.0
93.90	10416.0
94.90	81080.0
95.90	5185.0
96.80	137.0
103.80	492.0
104.70	172.0
105.70	489.0
110.70	138.0
111.80	101.0
115.80	363.0
116.80	702.0
117.80	335.0
118.80	439.0
127.80	310.0
128.90	149.0
129.80	301.0
134.80	171.0
136.80	189.0
140.90	849.0
141.80	122.0
142.80	1036.0
144.90	201.0
147.70	202.0
154.90	179.0
156.80	147.0
170.70	128.0
171.80	723.0
172.90	949.0
173.90	62488.0
174.90	4837.0
175.80	60592.0
176.90	4092.0

Instrument :
MSVOA_U
ClientSampleId :
BFB143