

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041619\
 Data File : VU031206.D
 Acq On : 16 Apr 2019 10:27
 Operator : JC/SP
 Sample : VU0416WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0416WBL01

Quant Time: Apr 17 03:09:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U041519DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Apr 16 04:55:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.74	96	28816	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	9736	0.92	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	10580	1.00	ug/l	0.00
Spiked Amount 1.000			Recovery	=	100.00%	


Target Compounds	Ovalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041619\
Data File : VU031206.D
Acq On : 16 Apr 2019 10:27
Operator : JC/SP
Sample : VU0416WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0416WBL01

Quant Time: Apr 17 03:09:13 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U041519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Apr 16 04:55:56 2019
Response via : Initial Calibration

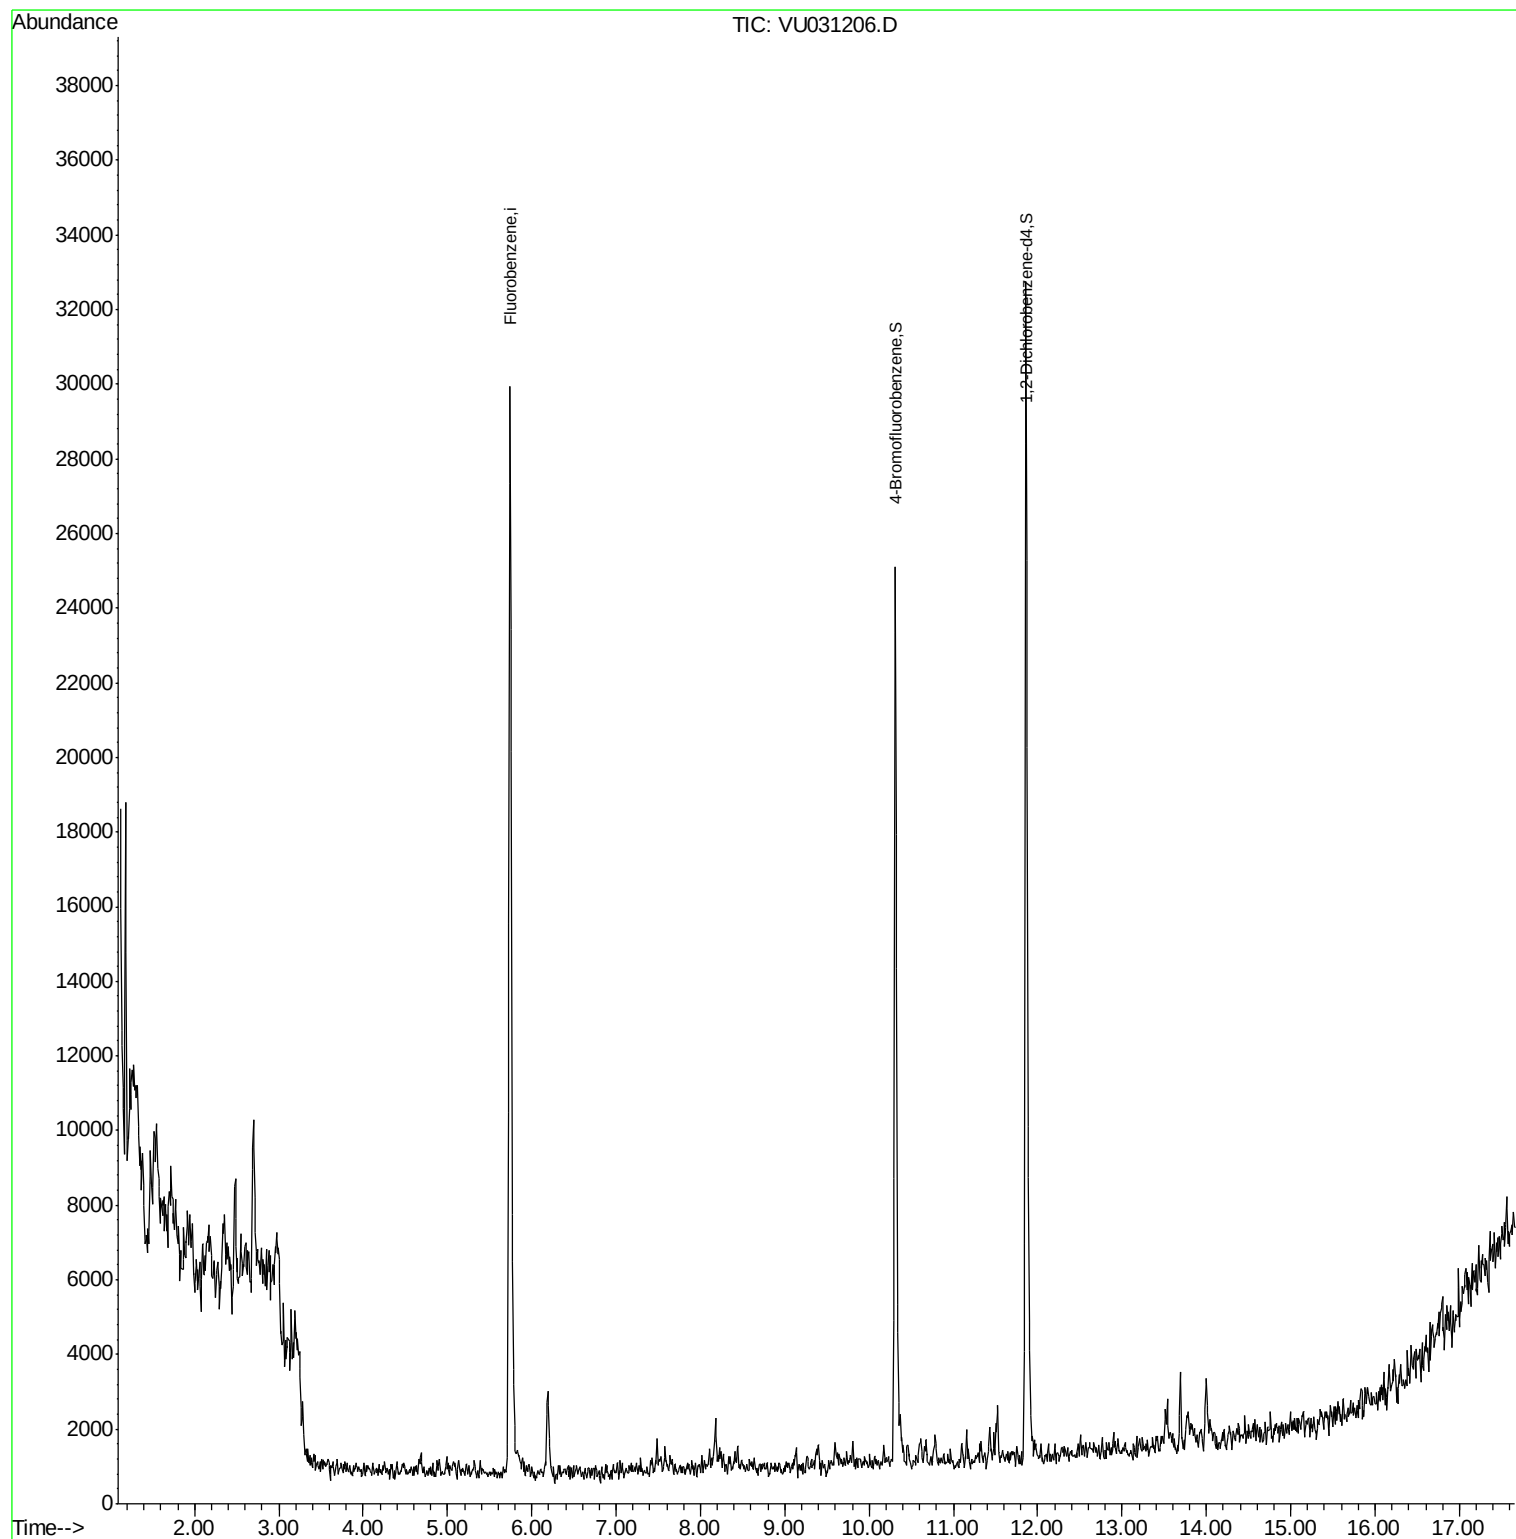

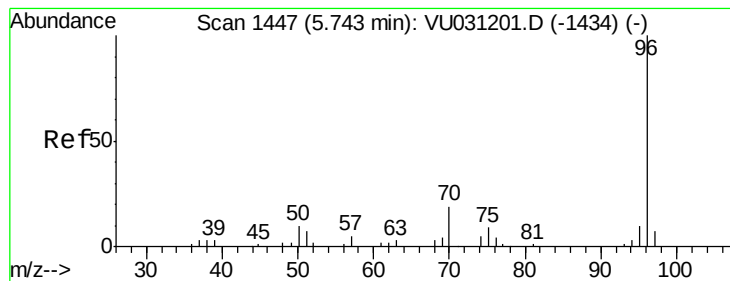

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1447

Delta R.T. 0.00 min

Lab File: VU031206.D

Acq: 16 Apr 2019 10:27

Instrument :

MSVOA_U

ClientSampleId :

VU0416WBL01

Tot Ion: 96 Resp: 28816


Ion Ratio Lower Upper

96 100

70 23.1 18.4 27.6

95 7.1 7.6 11.4#

97 6.5 0.0 0.0#



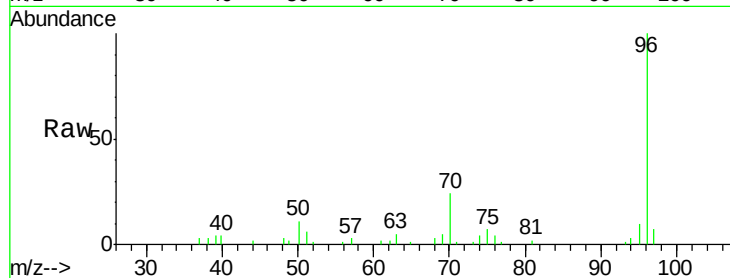


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

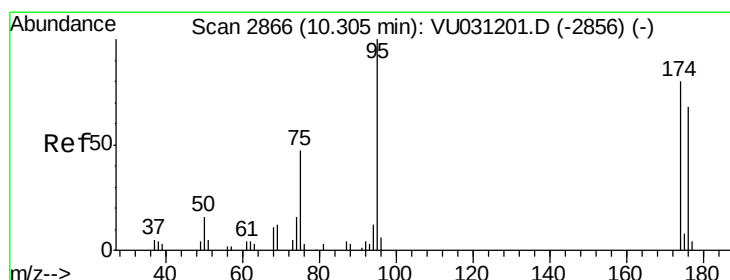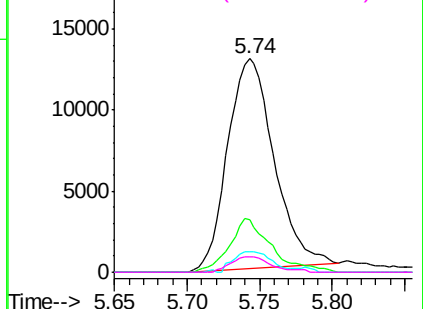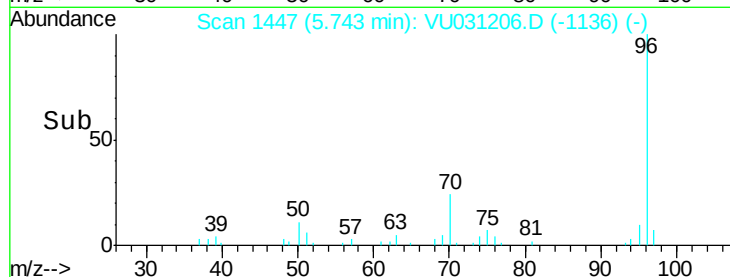

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2867

Delta R.T. 0.00 min

Lab File: VU031206.D

Acq: 16 Apr 2019 10:27


Tgt Ion: 95 Resp: 9736

Ion Ratio Lower Upper

95 100

174 90.1 64.2 96.2



176 82.8 58.0 87.0

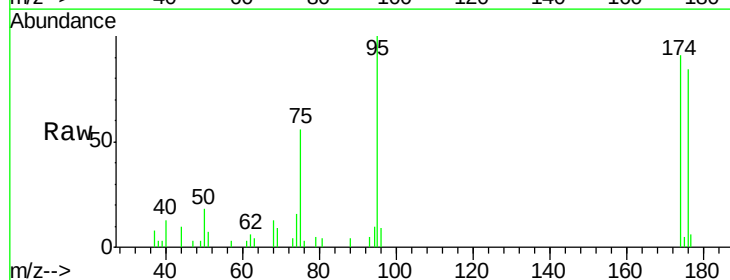


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

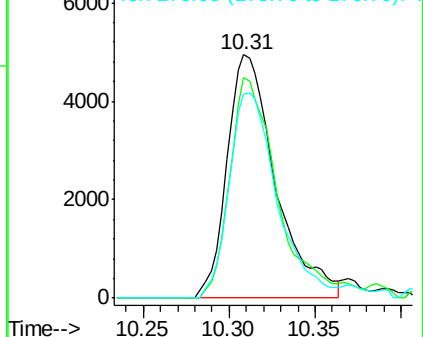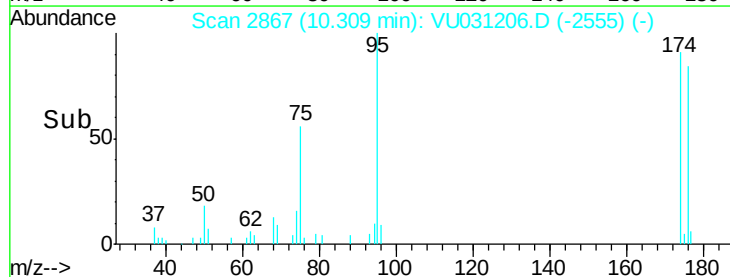

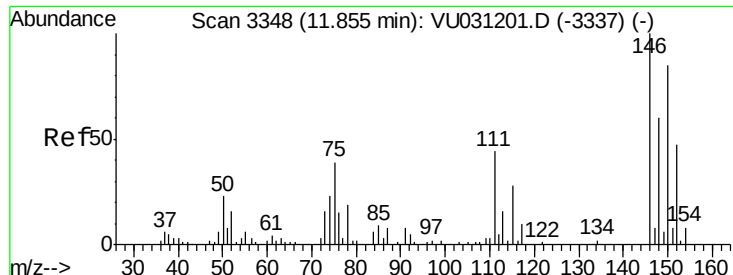

#68

1,2-Dichlorobenzene-d4

Concen: N.D. ug/l

RT: 11.86 min Scan# 3351

Delta R.T. 0.01 min

Lab File: VU031206.D

Acq: 16 Apr 2019 10:27

Instrument :

MSVOA_U

ClientSampleId :

VU0416WBL01


Tot Ion:152 Resp: 10580

Ion Ratio Lower Upper

152 100

115 66.7 0.0 130.0

150 159.8 0.0 639.0

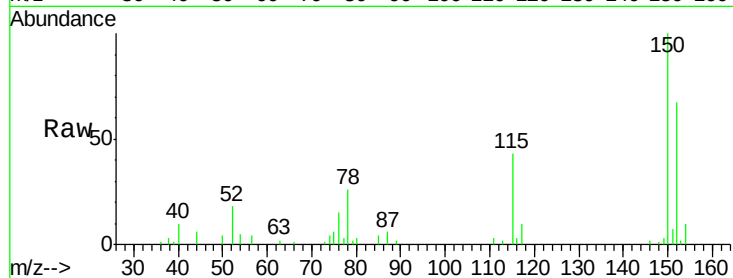

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

