

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041619\
 Data File : VU031206.D
 Acq On : 16 Apr 2019 10:27
 Operator : JC/SP
 Sample : VU0416WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0416WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.470	425	429	431	rBV2	2661	2147	3.35%	0.997%
2	2.695	492	499	512	rBV8	4639	10204	15.94%	4.740%
3	3.055	609	611	615	rVB5	1715	1111	1.73%	0.516%
4	3.148	636	640	644	rBV5	1623	1321	2.06%	0.614%
5	3.190	649	653	656	rBV6	1224	1075	1.68%	0.499%
6	5.743	1433	1447	1466	rBV2	29060	63278	98.82%	29.392%
7	6.190	1579	1586	1598	rVB4	2177	4239	6.62%	1.969%
8	7.486	1980	1989	1993	rBV4	905	1135	1.77%	0.527%
9	7.582	2012	2019	2024	rBV3	643	679	1.06%	0.315%
10	8.177	2196	2204	2212	rBV5	1211	1608	2.51%	0.747%
11	9.138	2500	2503	2507	rVB	824	692	1.08%	0.321%
12	9.395	2581	2583	2590	rVB4	659	681	1.06%	0.316%
13	10.309	2858	2867	2883	rBV2	23978	43997	68.71%	20.436%
14	10.781	3011	3014	3025	rVB3	817	1105	1.73%	0.513%
15	11.157	3126	3131	3135	rBV2	902	868	1.36%	0.403%
16	11.431	3210	3216	3221	rBV2	761	912	1.42%	0.424%
17	11.502	3235	3238	3241	rVV	908	773	1.21%	0.359%
18	11.524	3243	3245	3254	rVB3	1538	1079	1.69%	0.501%
19	11.862	3337	3350	3371	rBV3	31708	64035	100.00%	29.744%
20	13.209	3761	3769	3776	rBV3	540	978	1.53%	0.454%
21	13.534	3868	3870	3877	rVB4	1057	705	1.10%	0.327%
22	13.691	3912	3919	3924	rBV4	2115	2558	3.99%	1.188%
23	13.990	4006	4012	4013	rBV4	1621	1212	1.89%	0.563%
24	15.620	4515	4519	4521	rBV	729	646	1.01%	0.300%
25	15.881	4596	4600	4606	rBV4	798	1029	1.61%	0.478%
26	16.167	4681	4689	4691	rBV6	1225	1572	2.45%	0.730%
27	16.283	4722	4725	4728	rBV4	806	751	1.17%	0.349%
28	16.382	4753	4756	4760	rBV2	946	700	1.09%	0.325%
29	16.427	4766	4770	4773	rBV4	1038	954	1.49%	0.443%
30	16.646	4834	4838	4841	rBV3	1350	1044	1.63%	0.485%
31	16.990	4943	4945	4948	rVB3	1577	799	1.25%	0.371%
32	17.363	5056	5061	5064	rBV6	1276	1401	2.19%	0.651%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041619\
Data File : VU031206.D
Acq On : 16 Apr 2019 10:27
Operator : JC/SP
Sample : VU0416WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0416WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER


Sum of corrected areas: 215288

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041619\
Data File : VU031206.D
Acq On : 16 Apr 2019 10:27
Operator : JC/SP
Sample : VU0416WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0416WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U041519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

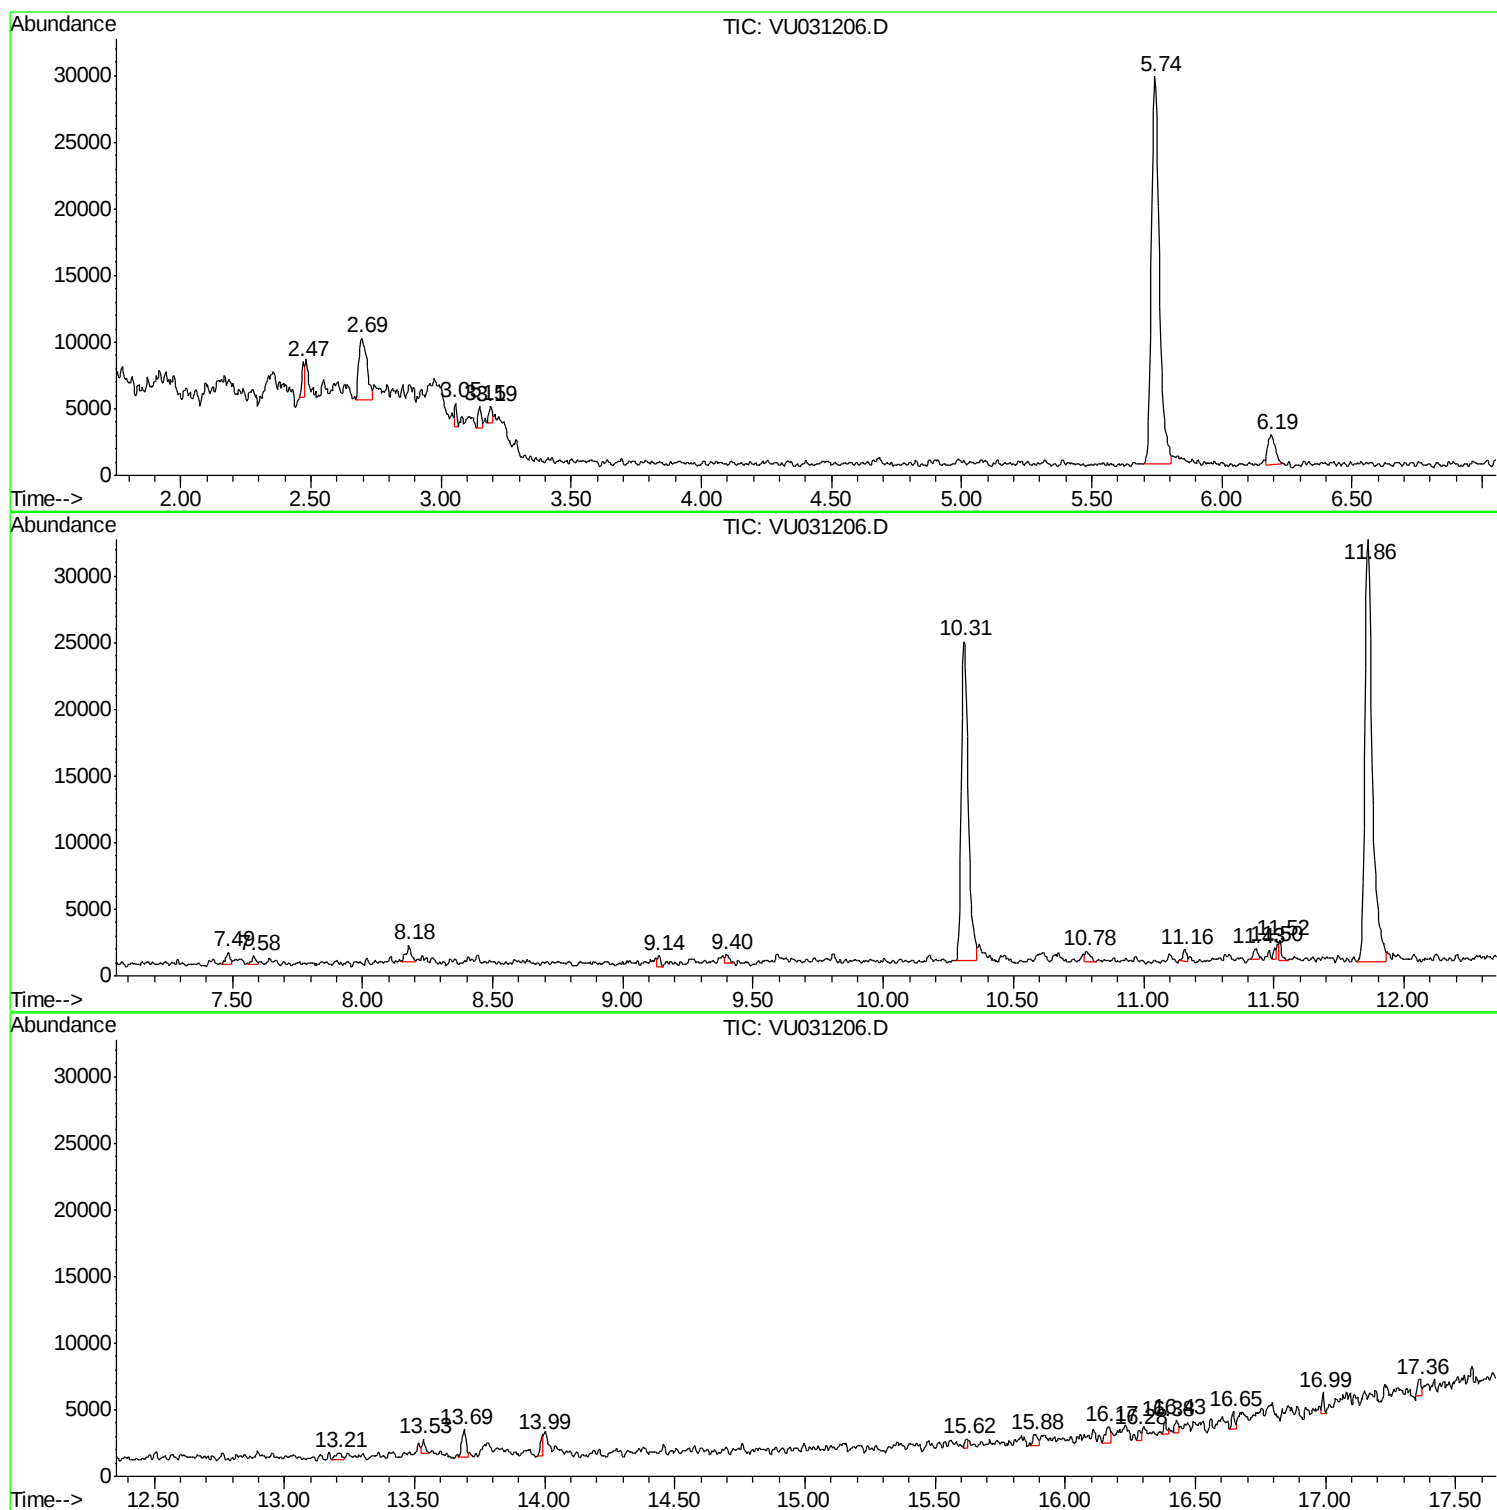

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041619\
Data File : VU031206.D
Acq On : 16 Apr 2019 10:27
Operator : JC/SP
Sample : VU0416WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0416WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041619\
Data File : VU031206.D
Acq On : 16 Apr 2019 10:27
Operator : JC/SP
Sample : VU0416WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0416WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc