


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041619\
Data File : VU031204.D
Acq On : 16 Apr 2019 09:25
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U041519DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Apr 16 04:55:56 2019

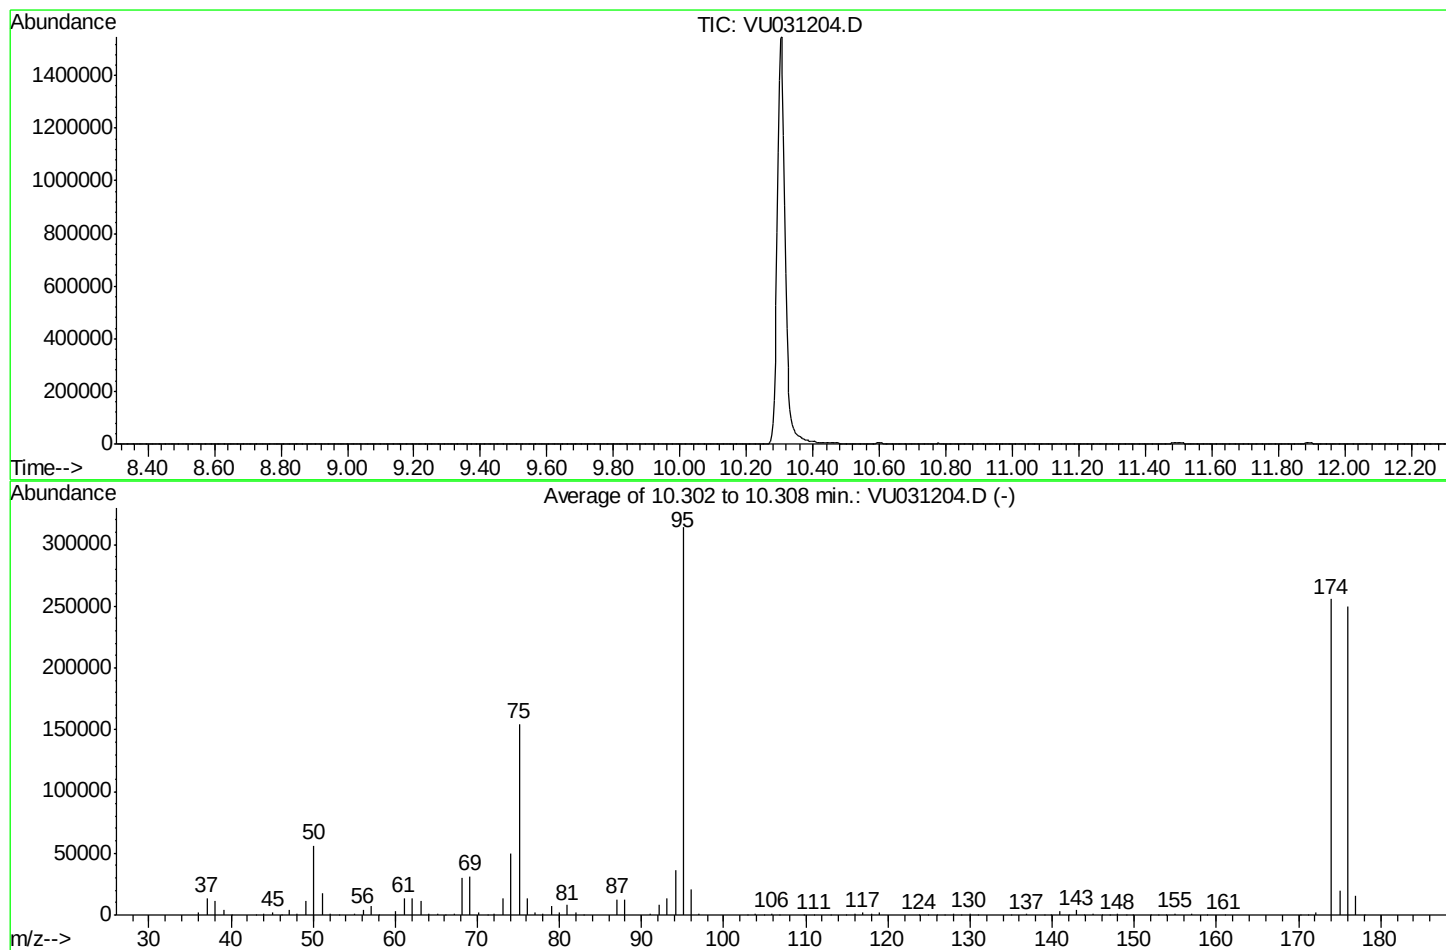

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	56149	PASS
75	95	30	60	49.3	154752	PASS
95	95	100	100	100.0	313813	PASS
96	95	5	9	6.5	20506	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.4	255573	PASS
175	174	5	9	7.6	19498	PASS
176	174	95	101	97.6	249450	PASS
177	176	5	9	6.3	15628	PASS