
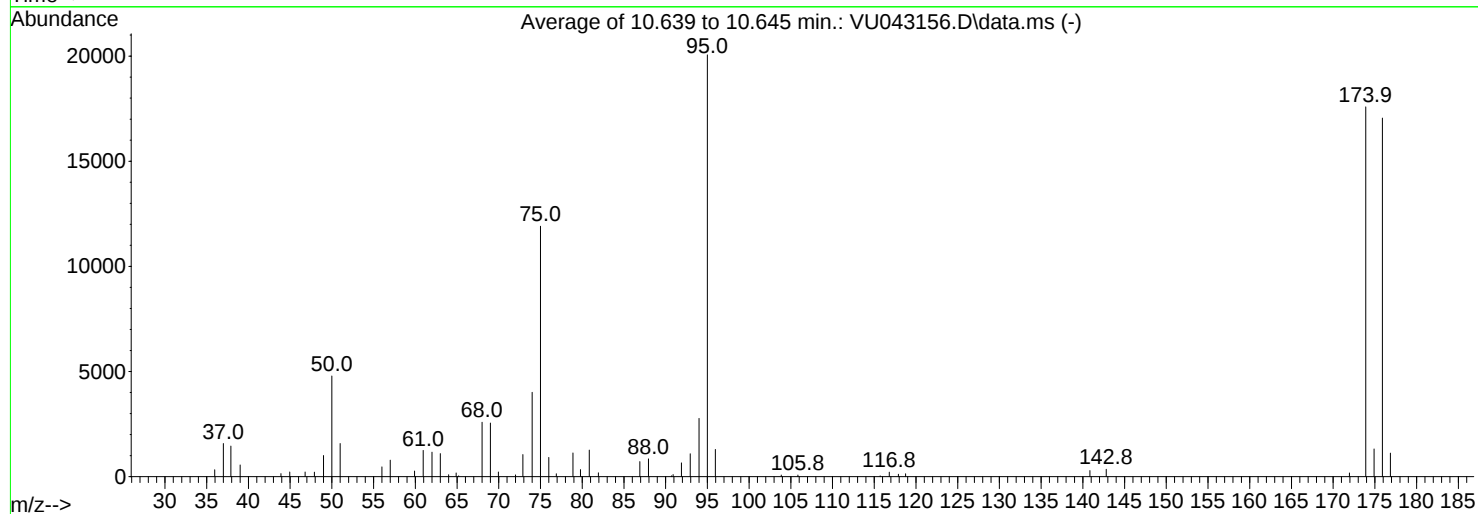


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041621\
 Data File : VU043156.D
 Acq On : 16 Apr 2021 08:58
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Title : SW846 8260
 Last Update : Mon Apr 12 13:17:29 2021

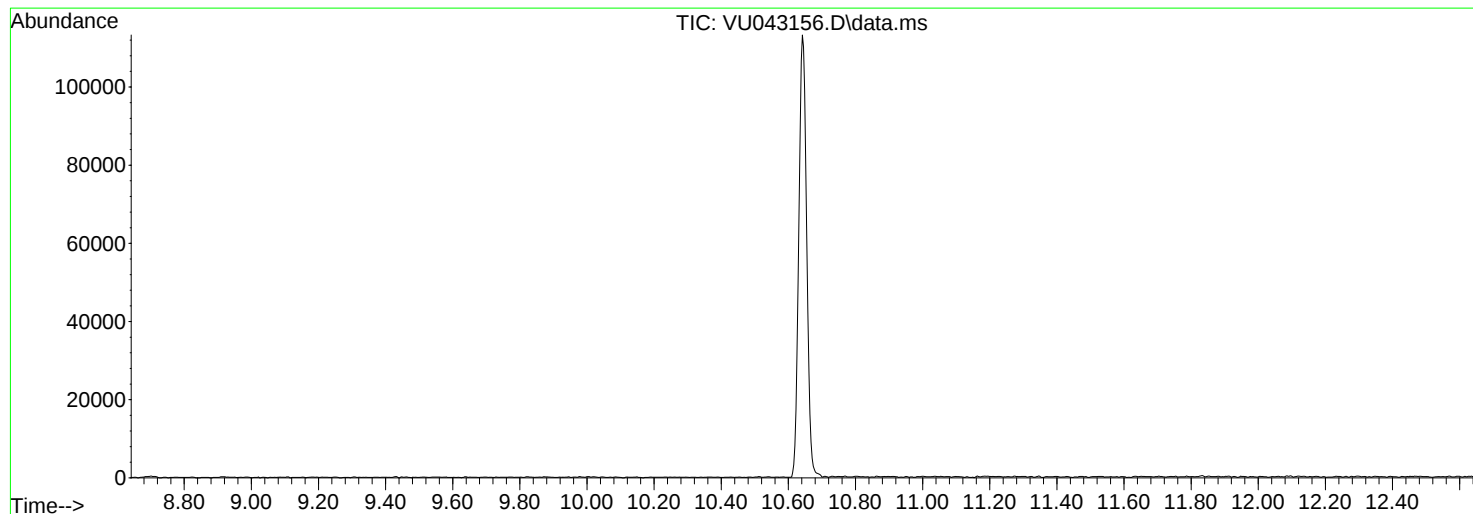

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	4785	PASS
75	95	30	60	59.4	11908	PASS
95	95	100	100	100.0	20059	PASS
96	95	5	9	6.4	1291	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.7	17587	PASS
175	174	5	9	7.5	1316	PASS
176	174	95	101	97.0	17055	PASS
177	176	5	9	6.5	1115	PASS