

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041719\
 Data File : VU031234.D
 Acq On : 17 Apr 2019 00:38
 Operator : JC/SP
 Sample : K2339-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB	59508	54867	0.56%	0.217%
2	1.299	61	65	75	rVB4	16150	15996	0.16%	0.063%
3	1.395	87	95	107	rBV	327622	375334	3.81%	1.483%
4	1.682	176	184	199	rVV	252807	307625	3.12%	1.216%
5	1.756	202	207	220	rVB2	36274	50097	0.51%	0.198%
6	2.273	357	368	382	rBV2	502387	799453	8.12%	3.159%
7	2.479	423	432	434	rBV6	1323	1665	0.02%	0.007%
8	2.704	494	502	509	rBV7	3276	6001	0.06%	0.024%
9	2.788	524	528	529	rBV4	909	611	0.01%	0.002%
10	2.839	540	544	549	rVB3	1376	1409	0.01%	0.006%
11	2.952	575	579	582	rBV4	841	781	0.01%	0.003%
12	2.990	582	591	592	rBV6	3094	3469	0.04%	0.014%
13	3.164	642	645	648	rVB2	876	607	0.01%	0.002%
14	3.190	648	653	654	rBV2	662	583	0.01%	0.002%
15	3.309	684	690	699	rVV6	1340	2161	0.02%	0.009%
16	3.447	721	733	743	rBV2	4897	10112	0.10%	0.040%
17	3.582	771	775	780	rVB3	806	827	0.01%	0.003%
18	3.694	806	810	815	rBV3	1149	1003	0.01%	0.004%
19	3.926	879	882	889	rVB3	580	597	0.01%	0.002%
20	3.971	891	896	899	rBV3	632	662	0.01%	0.003%
21	4.087	924	932	934	rBV6	1695	2187	0.02%	0.009%
22	4.218	949	973	999	rBV2	206316	885931	9.00%	3.501%
23	4.444	1039	1043	1045	rBV4	908	715	0.01%	0.003%
24	4.643	1087	1105	1130	rBV	315094	753542	7.65%	2.978%
25	4.762	1140	1142	1146	rBV2	866	574	0.01%	0.002%
26	4.907	1179	1187	1198	rVB10	4195	8715	0.09%	0.034%
27	4.990	1206	1213	1215	rBV6	1845	2132	0.02%	0.008%
28	5.058	1230	1234	1236	rBV2	984	587	0.01%	0.002%
29	5.074	1236	1239	1250	rVV7	1136	1481	0.02%	0.006%
30	5.337	1298	1321	1355	rVV2	637398	1945811	19.76%	7.689%
31	5.672	1421	1425	1430	rVV6	1132	1149	0.01%	0.005%
32	5.784	1453	1460	1463	rBV6	1469	1960	0.02%	0.008%
33	5.884	1477	1491	1522	rBV	568442	1202732	12.21%	4.753%
34	6.183	1568	1584	1617	rBV	5013008	9847860	100.00%	38.914%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041719\
 Data File : VU031234.D
 Acq On : 17 Apr 2019 00:38
 Operator : JC/SP
 Sample : K2339-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

35	6.328	1618	1629	1650	rVB	418899	871640	8.85%	3.444%
36	6.591	1708	1711	1716	rVB5	1855	1495	0.02%	0.006%
37	6.617	1716	1719	1725	rVB4	1227	689	0.01%	0.003%
38	6.649	1727	1729	1733	rVB3	1039	572	0.01%	0.002%
39	6.669	1733	1735	1737	rBV2	809	559	0.01%	0.002%
40	6.865	1792	1796	1799	rBV2	809	705	0.01%	0.003%
41	6.881	1799	1801	1803	rVV2	956	547	0.01%	0.002%
42	6.997	1833	1837	1839	rBV5	861	555	0.01%	0.002%
43	7.058	1853	1856	1862	rVB5	675	703	0.01%	0.003%
44	7.225	1892	1908	1938	rBV	227372	443579	4.50%	1.753%
45	7.382	1952	1957	1960	rBV5	772	659	0.01%	0.003%
46	7.424	1967	1970	1975	rVB3	924	678	0.01%	0.003%
47	7.562	1996	2013	2036	rBV	789858	1499457	15.23%	5.925%
48	7.849	2089	2102	2132	rVV2	149923	288676	2.93%	1.141%
49	7.977	2140	2142	2145	rVB3	1119	623	0.01%	0.002%
50	8.122	2182	2187	2188	rBV3	939	704	0.01%	0.003%
51	8.228	2214	2220	2229	rVB9	3357	4895	0.05%	0.019%
52	8.312	2234	2246	2285	rBV	549249	1086483	11.03%	4.293%
53	8.614	2335	2340	2343	rBV5	923	880	0.01%	0.003%
54	8.656	2350	2353	2355	rBV	980	657	0.01%	0.003%
55	8.749	2377	2382	2386	rBV4	873	1066	0.01%	0.004%
56	8.884	2417	2424	2426	rVB6	1007	968	0.01%	0.004%
57	8.964	2445	2449	2452	rBV4	788	610	0.01%	0.002%
58	9.086	2474	2487	2518	rBV	801170	1461916	14.85%	5.777%
59	9.257	2538	2540	2545	rVB3	1664	1138	0.01%	0.004%
60	9.379	2570	2578	2580	rBV5	1676	1869	0.02%	0.007%
61	9.447	2596	2599	2604	rVB3	1151	1097	0.01%	0.004%
62	9.472	2604	2607	2609	rBV2	813	606	0.01%	0.002%
63	10.238	2837	2845	2850	rBV3	633	921	0.01%	0.004%
64	10.283	2856	2859	2864	rBV2	736	605	0.01%	0.002%
65	10.376	2881	2888	2889	rBV2	773	819	0.01%	0.003%
66	10.427	2892	2904	2923	rBV	575796	935106	9.50%	3.695%
67	10.604	2952	2959	2974	rVB6	5355	9996	0.10%	0.039%
68	10.784	3012	3015	3021	rVB3	787	768	0.01%	0.003%
69	10.816	3021	3025	3029	rBV2	1115	640	0.01%	0.003%
70	10.839	3029	3032	3041	rVB3	907	989	0.01%	0.004%
71	10.926	3057	3059	3063	rVB2	882	579	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041719\
 Data File : VU031234.D
 Acq On : 17 Apr 2019 00:38
 Operator : JC/SP
 Sample : K2339-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC37

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis

72	10.951	3063	3067	3072	rBV5	722	710	0.01%	0.003%
73	11.064	3096	3102	3105	rBV2	542	578	0.01%	0.002%
74	11.167	3131	3134	3139	rVV4	809	688	0.01%	0.003%
75	11.324	3179	3183	3191	rVB4	1808	2245	0.02%	0.009%
76	11.482	3219	3232	3255	rBV	692135	1159404	11.77%	4.581%
77	11.762	3316	3319	3324	rVB5	958	826	0.01%	0.003%
78	11.858	3337	3349	3379	rBV	703356	1208216	12.27%	4.774%
79	12.228	3458	3464	3467	rBV4	1446	1544	0.02%	0.006%
80	12.356	3500	3504	3506	rBV3	1089	910	0.01%	0.004%
81	12.678	3601	3604	3608	rBV3	818	590	0.01%	0.002%
82	12.749	3622	3626	3631	rVB3	1317	1232	0.01%	0.005%
83	12.929	3678	3682	3686	rBV2	1136	1022	0.01%	0.004%
84	12.951	3686	3689	3693	rVV2	1035	1055	0.01%	0.004%
85	12.974	3693	3696	3699	rVB3	1386	897	0.01%	0.004%
86	13.003	3703	3705	3708	rBV2	851	626	0.01%	0.002%
87	13.061	3720	3723	3725	rBV2	887	609	0.01%	0.002%
88	13.102	3734	3736	3739	rVB3	1083	541	0.01%	0.002%
89	13.257	3780	3784	3788	rBV3	859	778	0.01%	0.003%
90	13.511	3860	3863	3867	rBV2	1060	678	0.01%	0.003%
91	13.668	3906	3912	3914	rBV2	797	832	0.01%	0.003%
92	13.813	3953	3957	3960	rBV4	779	772	0.01%	0.003%
93	13.858	3968	3971	3974	rBV	1035	699	0.01%	0.003%
94	13.938	3992	3996	4003	rVB3	985	1224	0.01%	0.005%
95	14.311	4109	4112	4114	rBV2	1497	906	0.01%	0.004%
96	14.482	4163	4165	4173	rVB3	1192	1382	0.01%	0.005%
97	14.639	4211	4214	4217	rBV2	1276	671	0.01%	0.003%
98	14.852	4276	4280	4286	rVB5	1142	1353	0.01%	0.005%
99	14.951	4309	4311	4314	rBV2	966	632	0.01%	0.002%
100	15.482	4473	4476	4481	rVB3	1578	1232	0.01%	0.005%


Sum of corrected areas: 25306537

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041719\
Data File : VU031234.D
Acq On : 17 Apr 2019 00:38
Operator : JC/SP
Sample : K2339-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

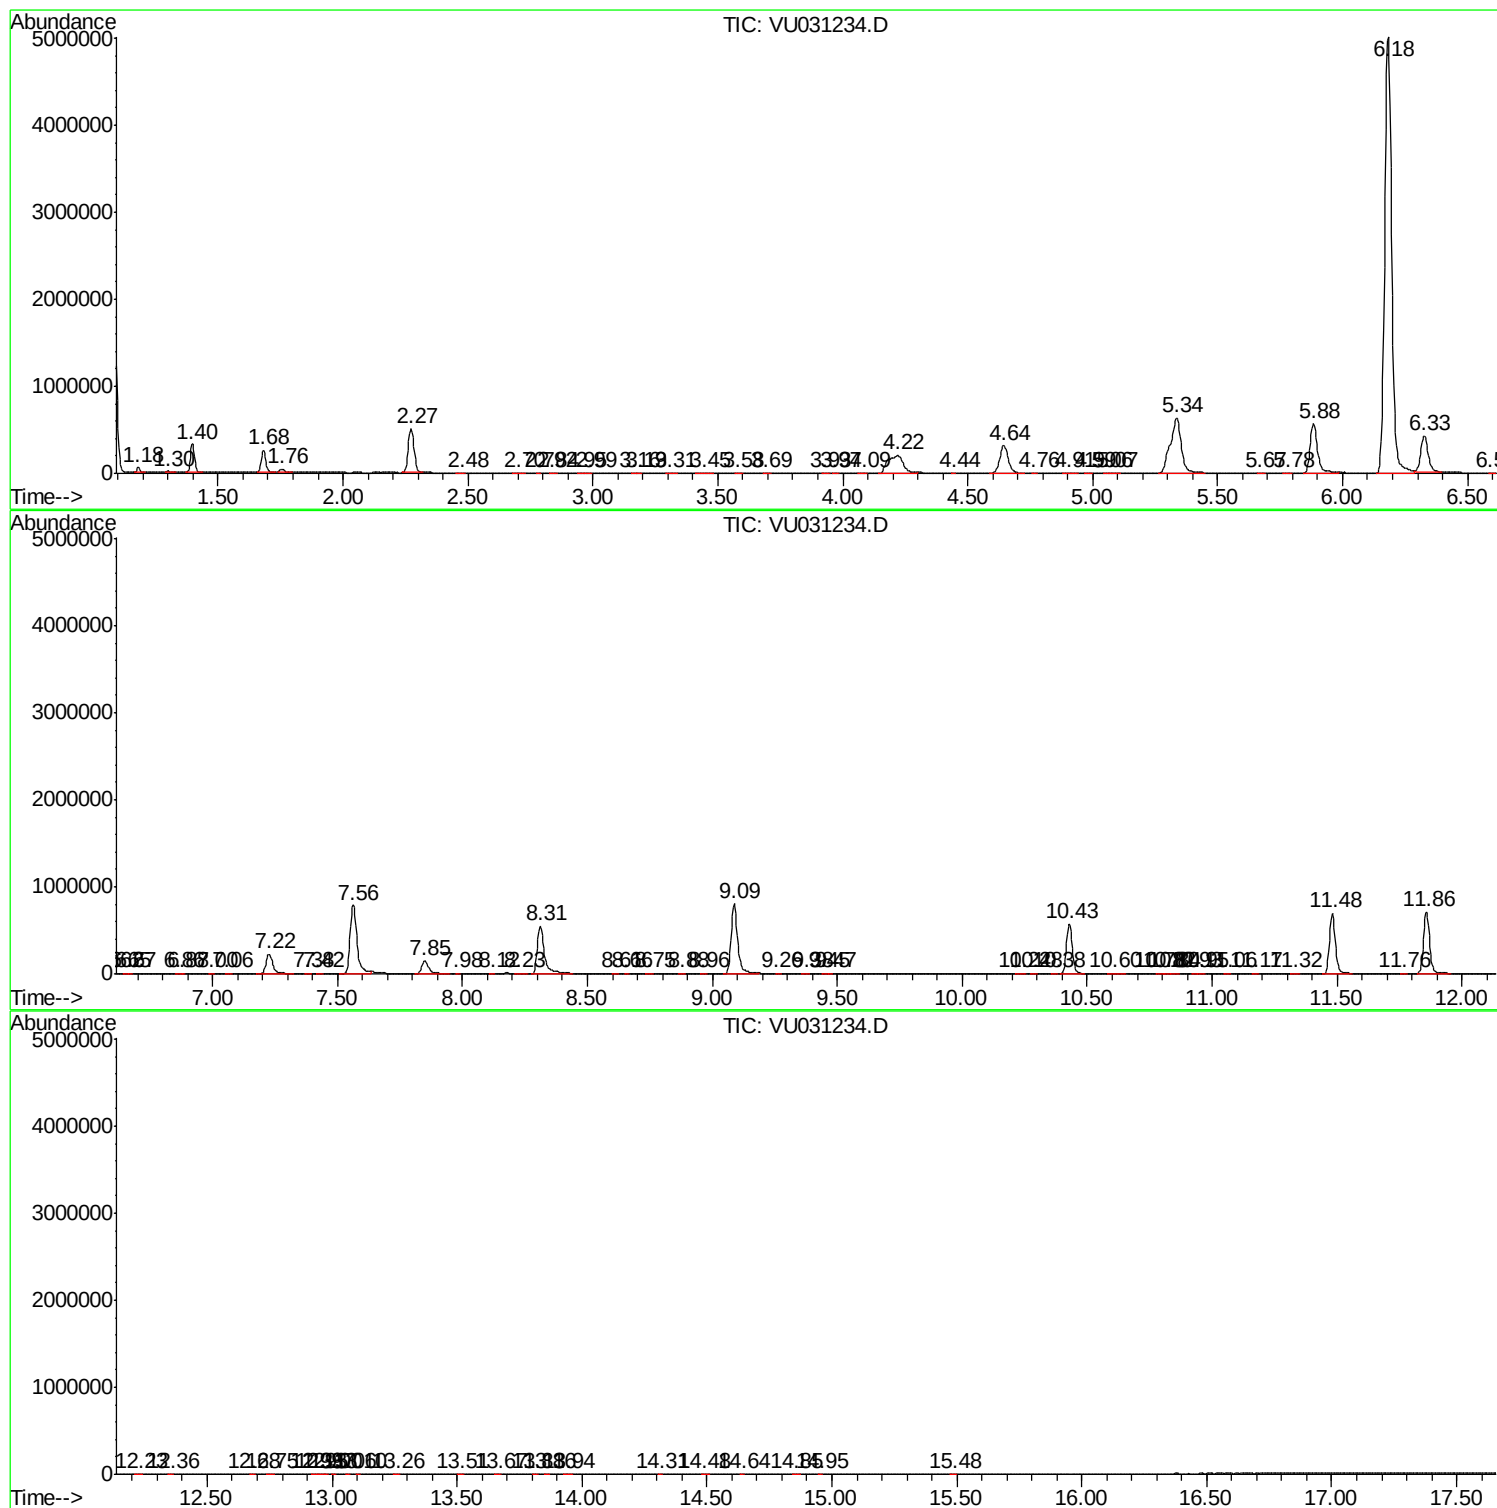

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041719\
Data File : VU031234.D
Acq On : 17 Apr 2019 00:38
Operator : JC/SP
Sample : K2339-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC37

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041719\
Data File : VU031234.D
Acq On : 17 Apr 2019 00:38
Operator : JC/SP
Sample : K2339-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC37

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
