


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041719\
 Data File : VU031212.D
 Acq On : 16 Apr 2019 14:39
 Operator : JC/SP
 Sample : BFB57
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB57

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 18 04:50:11 2019

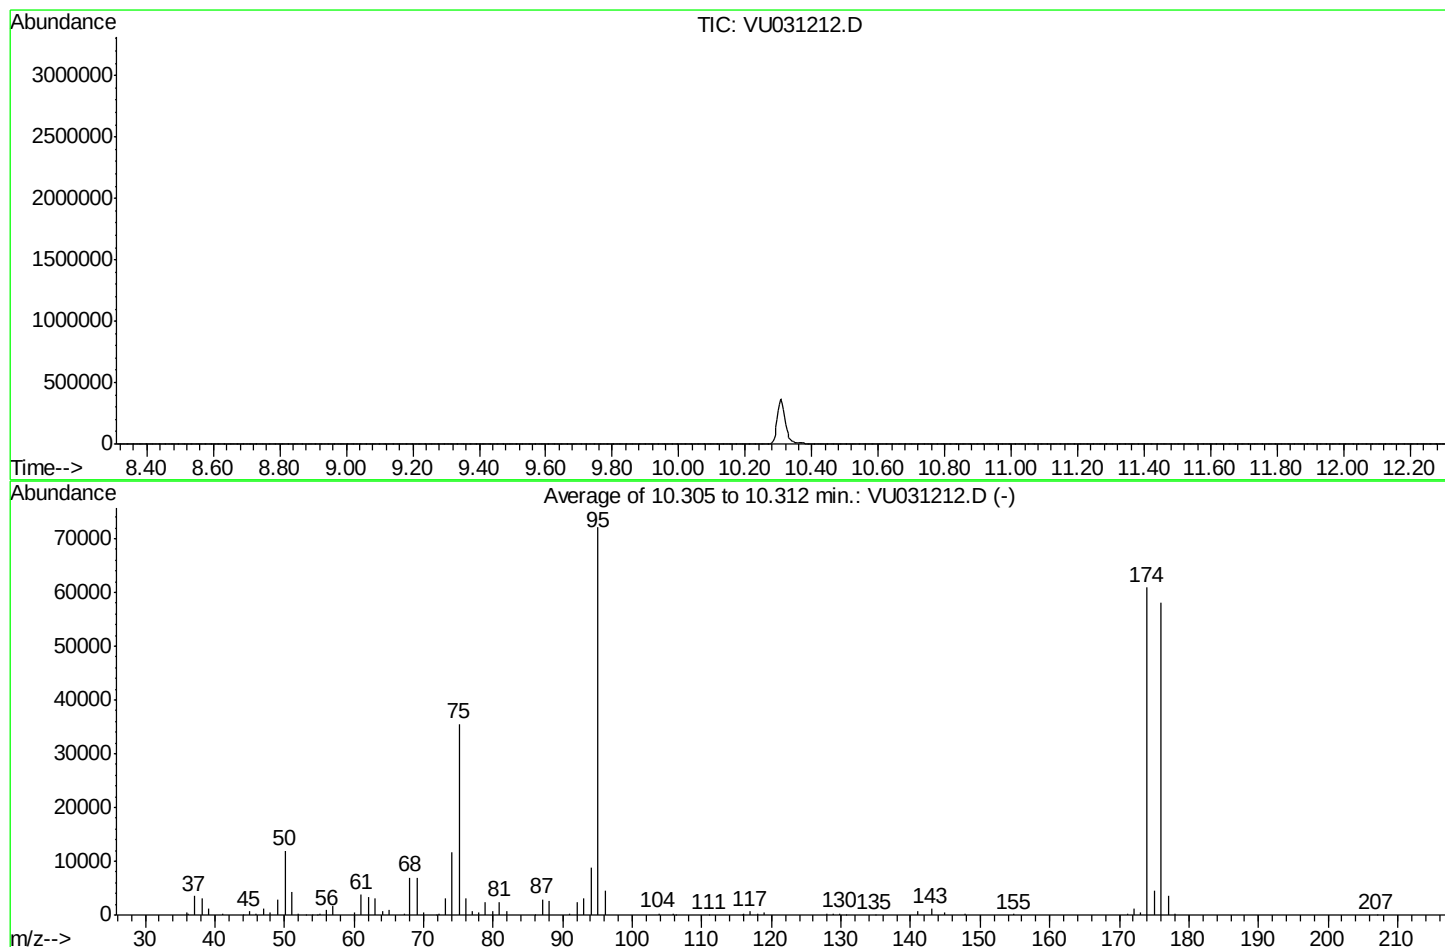

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	12013	PASS
75	95	30	80	49.2	35490	PASS
95	95	100	100	100.0	72090	PASS
96	95	5	9	6.4	4592	PASS
173	174	0.00	2	0.7	428	PASS
174	95	50	120	84.5	60893	PASS
175	174	5	9	7.3	4437	PASS
176	174	95	101	95.4	58114	PASS
177	176	5	9	6.1	3523	PASS

m/z	Abundance
36.10	604.0
37.00	3617.0
38.10	3076.0
39.10	1113.0
39.90	590.0
41.00	226.0
44.00	960.0
45.00	713.0
45.80	181.0
47.00	1229.0
48.00	566.0
49.00	2807.0
50.00	12188.0
51.10	4462.0
51.90	176.0
53.90	130.0
55.10	200.0
56.10	945.0
57.00	1733.0
60.00	501.0
61.00	3888.0
62.10	3320.0
63.10	3280.0
64.10	802.0
65.10	997.0
67.20	256.0
68.00	7254.0
69.10	7090.0
70.00	436.0
72.30	354.0
73.10	3275.0
74.10	11910.0
75.10	36264.0
76.10	3327.0
76.90	748.0
77.90	479.0
78.90	2272.0
80.00	720.0
80.90	2482.0
82.00	716.0
86.00	115.0
87.10	3027.0
88.00	2688.0
91.10	213.0
92.00	2627.0
93.10	3118.0
94.10	9112.0
95.10	74456.0
96.10	4707.0
103.90	297.0
105.80	232.0
116.00	187.0
117.00	698.0
118.00	224.0
119.00	486.0
127.90	252.0
129.00	169.0
129.80	266.0
130.70	144.0
134.80	120.0
140.90	770.0
143.00	1090.0
144.90	497.0
147.80	212.0
154.80	166.0
155.10	155.0
171.10	296.0
172.00	1164.0
174.00	62568.0
175.00	4491.0
176.00	60288.0
177.00	3683.0
178.00	269.0
207.00	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
35.90	720.0
37.00	3366.0
38.10	2677.0
39.10	916.0
39.90	546.0
41.00	120.0
44.00	883.0
45.00	633.0
45.80	251.0
47.00	1102.0
48.00	522.0
49.00	2758.0
50.10	11906.0
51.10	4100.0
51.90	129.0
55.10	225.0
56.10	811.0
57.00	1662.0
60.00	489.0
61.00	3527.0
62.10	3028.0
63.10	2907.0
64.10	736.0
65.10	968.0
67.20	351.0
68.00	6384.0
69.10	6476.0
70.00	412.0
71.90	325.0
73.10	2736.0
74.10	10655.0
75.10	33952.0
76.10	3029.0
76.90	622.0
77.80	315.0
78.80	2139.0
80.00	756.0
80.90	2275.0
82.00	544.0
87.00	2923.0
88.00	2557.0
91.00	204.0
92.00	2336.0
93.00	2666.0
94.10	8074.0
95.10	67904.0
96.10	4318.0
103.80	291.0
105.80	189.0
106.20	139.0
111.10	110.0
116.00	199.0
116.90	562.0
118.00	167.0
119.00	484.0
128.00	271.0
129.00	199.0
129.80	264.0
134.90	103.0
140.90	842.0
143.00	932.0
144.80	411.0
147.80	257.0
154.80	146.0
171.10	225.0
172.10	1137.0
174.00	59296.0
175.00	4082.0
176.00	55840.0
177.00	3163.0
177.90	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

Scan 2854 (10.267 min): VU031212.D
BFB57

m/z	Abundance
39.90	776.0
44.10	905.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57

m/z	Abundance
35.90	504.0
37.00	3516.0
38.10	3302.0
39.10	1234.0
39.90	708.0
41.10	264.0
43.90	959.0
44.90	701.0
45.90	119.0
47.00	1050.0
48.00	465.0
49.00	2681.0
50.00	11946.0
51.10	4446.0
51.90	258.0
53.00	139.0
54.00	115.0
54.80	186.0
56.10	939.0
57.00	1764.0
60.00	525.0
61.00	3707.0
62.00	3484.0
63.00	3245.0
64.10	701.0
65.10	812.0
67.10	134.0
68.00	7201.0
69.10	7009.0
70.00	519.0
72.20	372.0
73.10	3481.0
74.10	12194.0
75.10	36256.0
76.10	3156.0
76.90	651.0
77.90	540.0
79.00	2436.0
79.90	706.0
80.90	2609.0
82.00	797.0
85.90	129.0
87.10	2888.0
88.00	2653.0
91.10	256.0
92.00	2376.0
93.10	3263.0
94.10	9269.0
95.10	73912.0
96.10	4751.0
103.90	275.0
105.80	337.0
115.80	187.0
117.10	726.0
118.00	224.0
119.00	434.0
127.90	199.0
128.90	116.0
129.90	258.0
130.70	146.0
134.80	102.0
141.00	692.0
143.00	1228.0
145.00	540.0
147.80	214.0
155.00	170.0
171.10	236.0
172.00	987.0
173.10	1284.0
174.00	60816.0
175.00	4739.0
176.00	58216.0
177.00	3725.0
178.00	288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB57