


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041719\
 Data File : VU031244.D
 Acq On : 17 Apr 2019 08:25
 Operator : JC/SP
 Sample : BFB58
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB58

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 18 04:50:11 2019

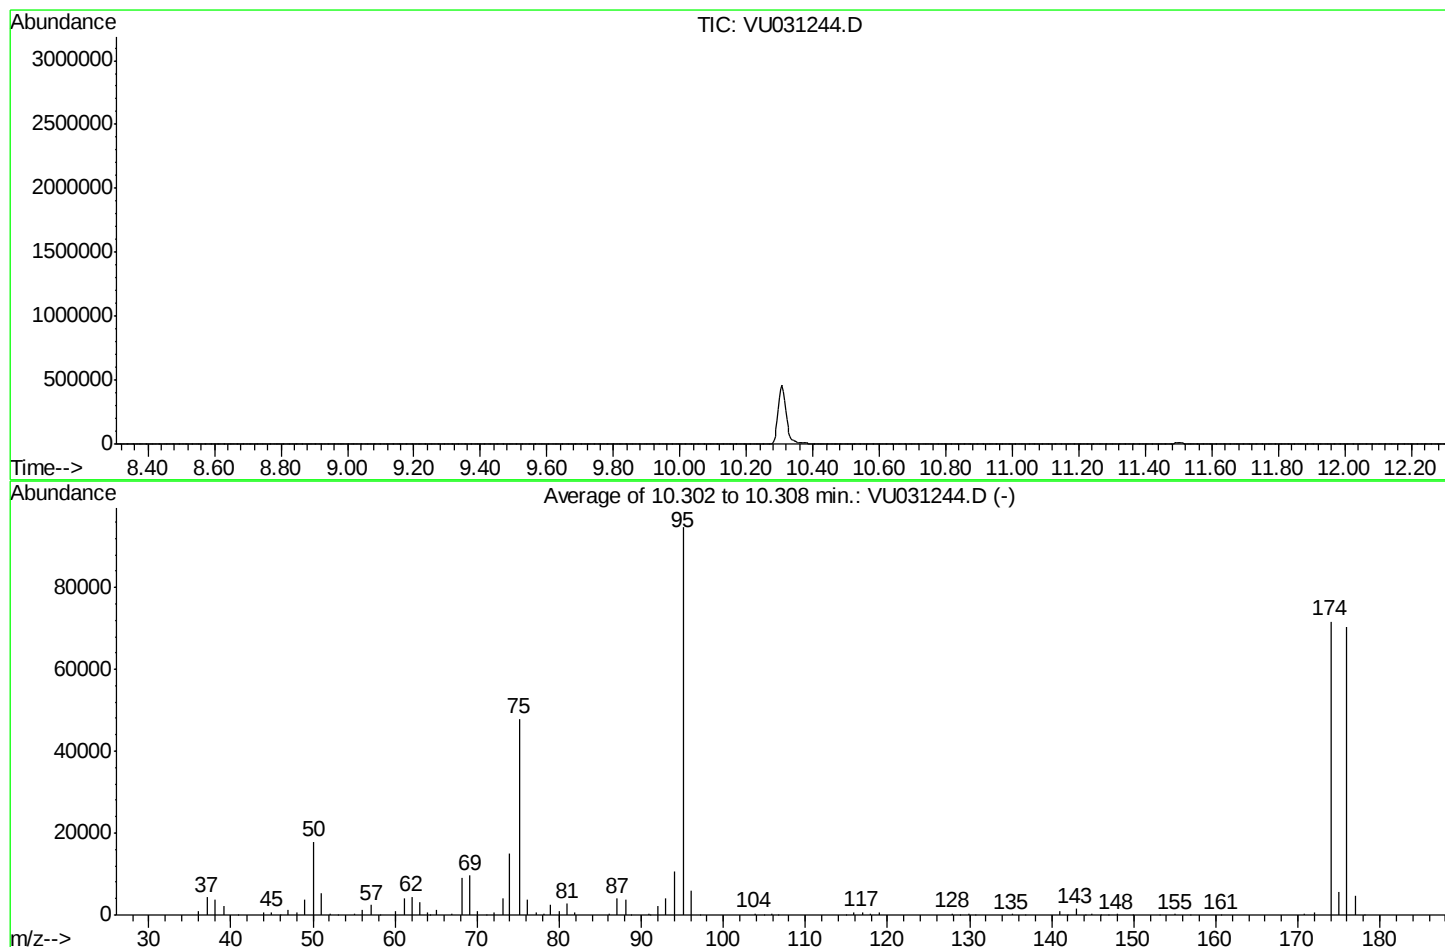

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	17826	PASS
75	95	30	80	50.5	47856	PASS
95	95	100	100	100.0	94682	PASS
96	95	5	9	6.3	6008	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	71642	PASS
175	174	5	9	8.0	5736	PASS
176	174	95	101	98.4	70506	PASS
177	176	5	9	6.7	4724	PASS

Scan 2853 (10.263 min): VU031244.D
BFB58

m/z	Abundance
40.00	1055.0
43.90	633.0
207.00	281.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.10	826.0
37.10	4041.0
38.00	3621.0
39.10	2120.0
40.00	921.0
44.10	1152.0
44.90	689.0
47.00	1399.0
48.00	746.0
49.00	3343.0
50.10	17688.0
51.00	5088.0
52.00	339.0
54.90	301.0
56.00	1386.0
57.10	2427.0
58.20	138.0
60.00	879.0
61.10	3945.0
62.10	4181.0
63.00	3018.0
64.00	448.0
64.20	454.0
65.10	961.0
66.90	282.0
68.10	8960.0
69.10	8966.0
70.10	696.0
71.10	120.0
72.10	496.0
73.10	3784.0
74.00	14143.0
75.10	45624.0
76.10	3899.0
77.20	417.0
78.10	487.0
79.00	2298.0
80.00	1057.0
81.00	2678.0
82.00	481.0
86.10	156.0
87.10	4067.0
88.10	3530.0
88.80	307.0
90.80	294.0
92.00	2050.0
93.00	3724.0
94.10	9787.0
95.10	92600.0
96.10	5885.0
97.30	102.0
103.90	426.0
105.90	355.0
115.00	111.0
116.00	509.0
116.90	652.0
118.00	408.0
119.00	467.0
127.90	307.0
129.90	230.0
130.80	139.0
135.20	166.0
136.80	101.0
141.00	833.0
142.00	143.0
143.00	1518.0
144.10	127.0
144.90	344.0
145.90	222.0
147.00	130.0
148.00	182.0
149.90	150.0
155.00	253.0
170.80	210.0
172.00	574.0
174.00	67096.0
175.00	5741.0
176.00	66304.0
177.00	4068.0
178.10	101.0
207.30	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.10	939.0
37.10	4362.0
38.00	3831.0
39.10	2142.0
40.00	909.0
44.10	1255.0
45.00	808.0
46.00	132.0
47.00	1461.0
48.00	816.0
49.10	3858.0
50.10	18328.0
51.10	5368.0
52.00	264.0
53.10	105.0
55.00	390.0
56.00	1198.0
57.10	2601.0
58.20	139.0
60.00	959.0
61.10	4348.0
62.10	4696.0
63.00	3171.0
63.90	531.0
65.10	1111.0
66.90	376.0
68.10	9496.0
69.10	9935.0
70.10	904.0
72.10	602.0
73.10	4255.0
74.00	15634.0
75.10	49416.0
76.10	3901.0
77.10	518.0
78.10	396.0
78.90	2403.0
80.00	977.0
81.00	2789.0
81.90	662.0
86.10	220.0
87.10	4126.0
88.10	3909.0
90.90	276.0
92.00	2375.0
93.00	4158.0
94.10	10980.0
95.10	97912.0
96.10	6162.0
97.10	138.0
103.80	483.0
105.00	118.0
105.80	364.0
106.70	108.0
115.90	532.0
116.90	715.0
117.90	489.0
119.00	524.0
127.90	350.0
129.90	194.0
130.70	109.0
135.10	214.0
136.80	164.0
141.00	987.0
142.00	124.0
143.00	1587.0
144.90	408.0
146.00	161.0
147.00	157.0
147.90	193.0
149.90	182.0
155.00	238.0
156.90	124.0
160.70	156.0
170.80	189.0
172.00	643.0
174.00	74032.0
175.00	5884.0
176.00	72560.0
177.00	4922.0
178.10	136.0
207.10	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58

m/z	Abundance
36.00	894.0
37.00	4296.0
38.00	3701.0
39.10	2072.0
39.90	895.0
40.80	115.0
44.10	1345.0
45.00	811.0
46.00	163.0
47.00	1352.0
48.00	659.0
49.10	3862.0
50.10	17464.0
51.10	5269.0
52.10	232.0
53.10	114.0
55.10	465.0
56.00	1040.0
57.10	2475.0
58.10	102.0
60.10	950.0
61.10	4355.0
62.00	4575.0
63.00	3253.0
64.00	499.0
65.00	1259.0
67.00	393.0
68.10	9153.0
69.10	9939.0
70.10	927.0
72.10	591.0
73.10	4100.0
74.00	15279.0
75.10	48528.0
76.10	3565.0
77.10	587.0
78.10	267.0
78.90	2476.0
79.90	845.0
81.00	2777.0
81.90	697.0
86.10	208.0
87.10	3842.0
88.10	3752.0
91.10	310.0
92.00	2487.0
93.00	4233.0
94.10	11566.0
95.10	93536.0
96.10	5978.0
97.10	183.0
103.90	438.0
104.90	141.0
105.80	329.0
115.00	117.0
115.90	484.0
116.90	710.0
117.90	443.0
119.00	529.0
127.90	398.0
128.90	133.0
129.90	214.0
135.10	188.0
136.90	189.0
141.00	953.0
143.00	1452.0
144.90	444.0
146.10	119.0
146.90	141.0
147.90	196.0
150.00	170.0
153.10	104.0
155.10	241.0
157.00	168.0
160.70	197.0
170.90	126.0
172.00	774.0
174.00	73800.0
175.10	5583.0
176.00	72656.0
177.00	5184.0
178.10	148.0
207.00	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB58