

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
 Data File : VU053733.D
 Acq On : 17 Apr 2023 17:44
 Operator : JC/MD
 Sample : 02340-06DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 MSVOA_U
 ClientSampleId :
 BHE08DL

Quant Time: Apr 18 00:22:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR0


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053733.D
Acq On : 17 Apr 2023 17:44
Operator : JC/MD
Sample : 02340-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Time: Apr 18 00:22:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE

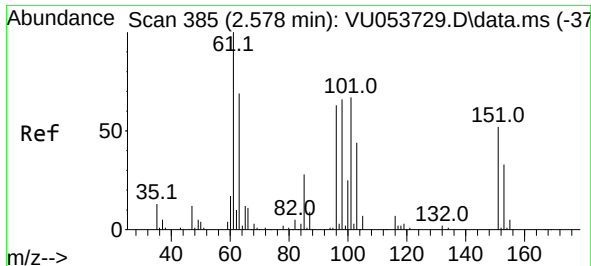


#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.199 ug/L
 RT: 2.572 min Scan# 383
 Delta R.T. -0.006 min
 Lab File: VU053733.D
 Acq: 17 Apr 2023 17:44

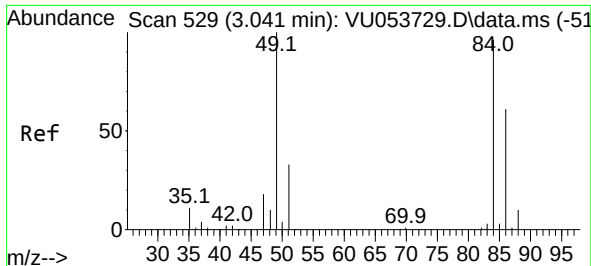

#16
Methylene chloride
Concen: 0.303 ug/L
RT: 3.038 min Scan# 51
Delta R.T. -0.003 min
Lab File: VU053733.D
Acq: 17 Apr 2023 17:44

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Tgt Ion: 84 Resp: 2985
Ion Ratio Lower Upper
84 100
86 6

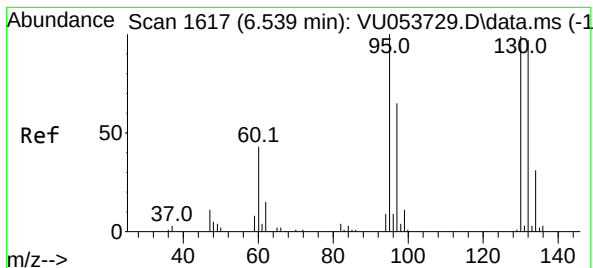

#34

Trichloroethene

Concen: 3.827 ug/L

RT: 6.539 min Scan# 1

Delta R.T. 0.000 min