

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
 Data File : VU053733.D
 Acq On : 17 Apr 2023 17:44
 Operator : JC/MD
 Sample : 02340-06DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE08DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	58616	71762	8.39%	1.645%
2	1.909	169	177	197	rVB	47897	67098	7.84%	1.538%
3	2.565	369	381	395	rBV	92977	157206	18.38%	3.603%
4	3.041	518	529	544	rVB2	5614	10124	1.18%	0.232%
5	4.623	1009	1021	1050	rBV	36964	106574	12.46%	2.443%
6	5.057	1141	1156	1177	rBV2	77365	171401	20.04%	3.929%
7	5.719	1340	1362	1391	rBV3	147350	383629	44.85%	8.793%
8	6.244	1509	1525	1544	rBV	155361	299018	34.96%	6.854%
9	6.539	1604	1617	1633	rBV	102142	190957	22.32%	4.377%
10	6.687	1650	1663	1678	rBV	90583	177385	20.74%	4.066%
11	7.562	1924	1935	1950	rBV2	36061	63417	7.41%	1.454%
12	7.893	2024	2038	2069	rBV	189254	334553	39.11%	7.668%
13	8.176	2116	2126	2142	rBV2	21771	36607	4.28%	0.839%
14	8.549	2228	2242	2257	rBV	506351	855429	100.00%	19.607%
15	8.629	2257	2267	2304	rVB	160384	303268	35.45%	6.951%
16	9.414	2498	2511	2532	rBV	218308	365936	42.78%	8.387%
17	10.751	2915	2927	2938	rBV	66796	108017	12.63%	2.476%
18	11.809	3244	3256	3273	rBV	229813	368392	43.07%	8.444%
19	12.189	3362	3374	3397	rBV2	173641	292104	34.15%	6.695%




Sum of corrected areas: 4362877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053733.D
Acq On : 17 Apr 2023 17:44
Operator : JC/MD
Sample : 02340-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

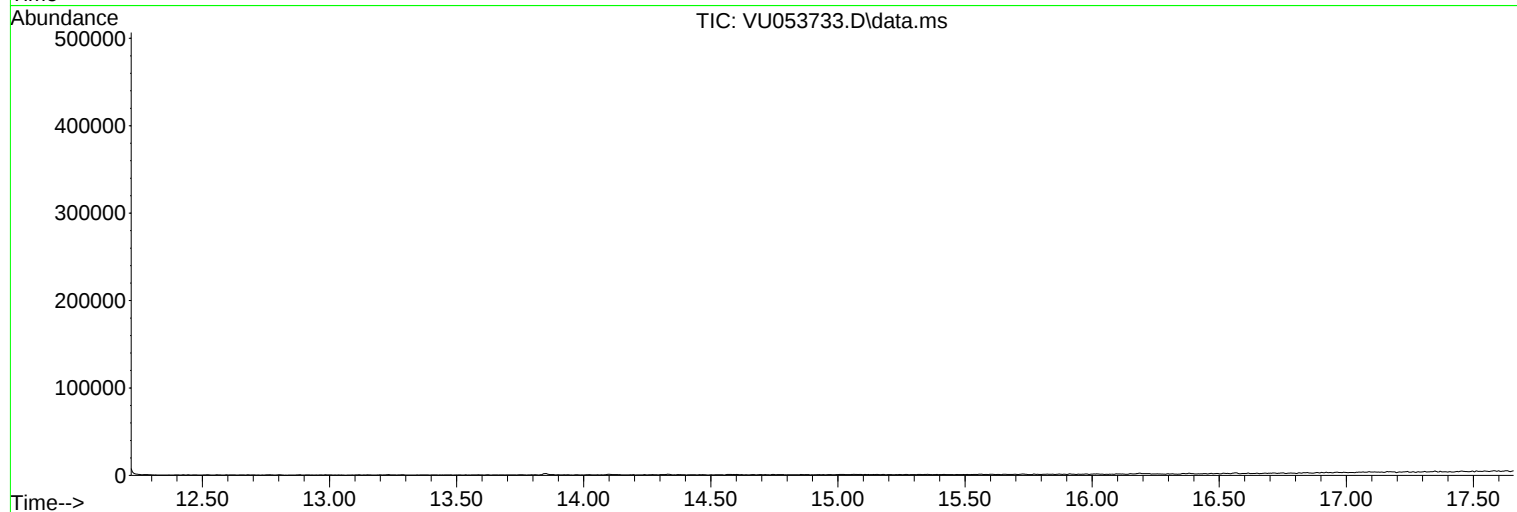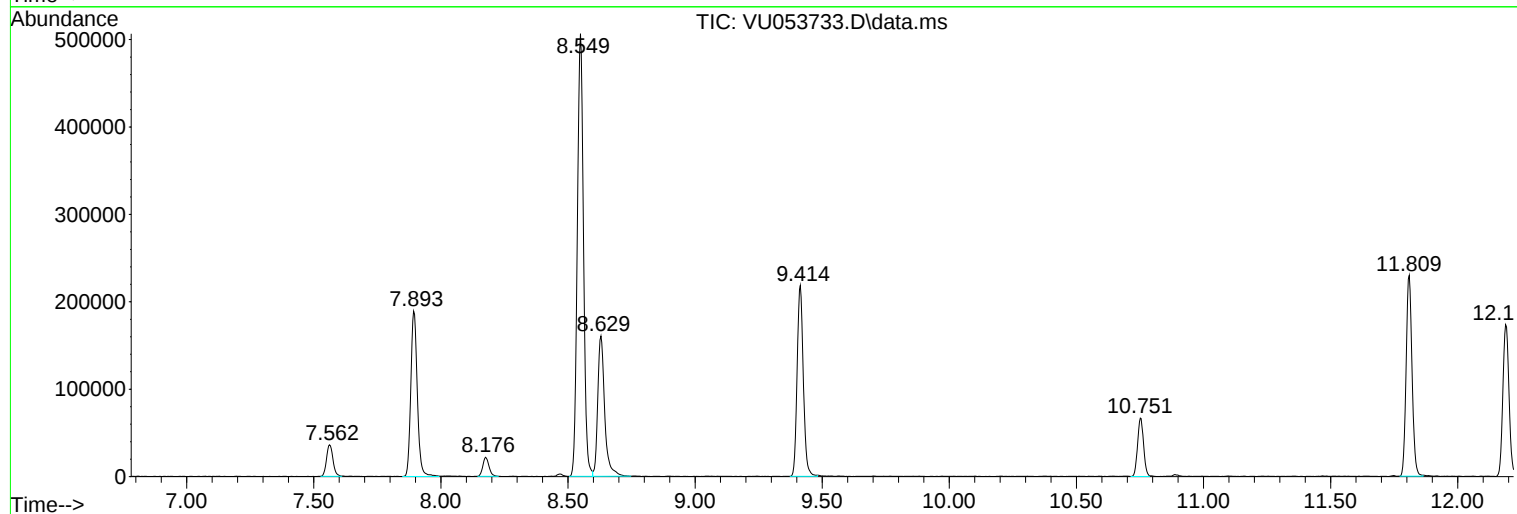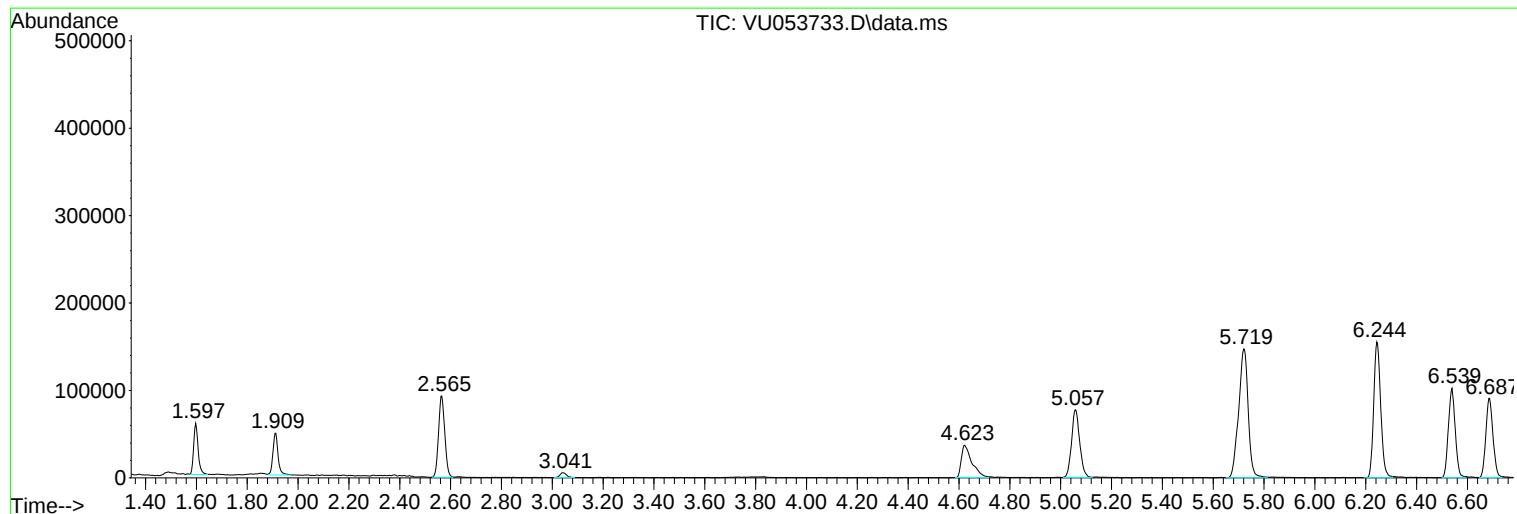

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053733.D
Acq On : 17 Apr 2023 17:44
Operator : JC/MD
Sample : 02340-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053733.D
Acq On : 17 Apr 2023 17:44
Operator : JC/MD
Sample : 02340-06DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE08DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc