

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
 Data File : VU053741.D
 Acq On : 17 Apr 2023 21:00
 Operator : JC/MD
 Sample : 02340-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE17

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	70	80	94	rVB	64045	85295	18.89%	2.114%
2	1.684	99	107	120	rBV2	8654	14011	3.10%	0.347%
3	1.912	170	178	196	rVB	54803	74956	16.60%	1.858%
4	2.565	365	381	394	rBV	94024	156177	34.59%	3.870%
5	2.633	394	402	414	rVB2	2929	5315	1.18%	0.132%
6	4.623	1009	1021	1047	rBV	66595	166008	36.77%	4.114%
7	5.057	1138	1156	1177	rBV	92398	209201	46.33%	5.184%
8	5.719	1343	1362	1385	rBV2	170726	451498	100.00%	11.189%
9	6.243	1511	1525	1551	rBV	163352	315071	69.78%	7.808%
10	6.687	1649	1663	1684	rBV	111445	215773	47.79%	5.347%
11	7.562	1923	1935	1949	rBV2	56081	97251	21.54%	2.410%
12	7.896	2025	2039	2053	rBV	215094	378958	83.93%	9.391%
13	7.967	2053	2061	2079	rVB	14528	27587	6.11%	0.684%
14	8.176	2115	2126	2140	rBV3	32762	54864	12.15%	1.360%
15	8.468	2206	2217	2226	rBV4	5843	10231	2.27%	0.254%
16	8.629	2253	2267	2293	rBV	234021	426461	94.45%	10.569%
17	8.835	2322	2331	2342	rVB2	5538	9017	2.00%	0.223%
18	9.414	2499	2511	2533	rBV	230744	387239	85.77%	9.597%
19	9.690	2588	2597	2608	rBV4	4592	7168	1.59%	0.178%
20	10.082	2711	2719	2723	rBV3	3440	5315	1.18%	0.132%
21	10.751	2915	2927	2948	rVB	87801	139597	30.92%	3.460%
22	10.889	2960	2970	2983	rVB4	8780	14587	3.23%	0.361%
23	11.468	3140	3150	3157	rBV3	3356	4848	1.07%	0.120%
24	11.510	3157	3163	3172	rVB3	4225	5757	1.28%	0.143%
25	11.809	3240	3256	3274	rBV	239334	391827	86.78%	9.710%
26	12.188	3362	3374	3398	rBV	220704	360237	79.79%	8.928%
27	12.886	3582	3591	3601	rBV5	13867	20888	4.63%	0.518%




Sum of corrected areas: 4035137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053741.D
Acq On : 17 Apr 2023 21:00
Operator : JC/MD
Sample : 02340-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

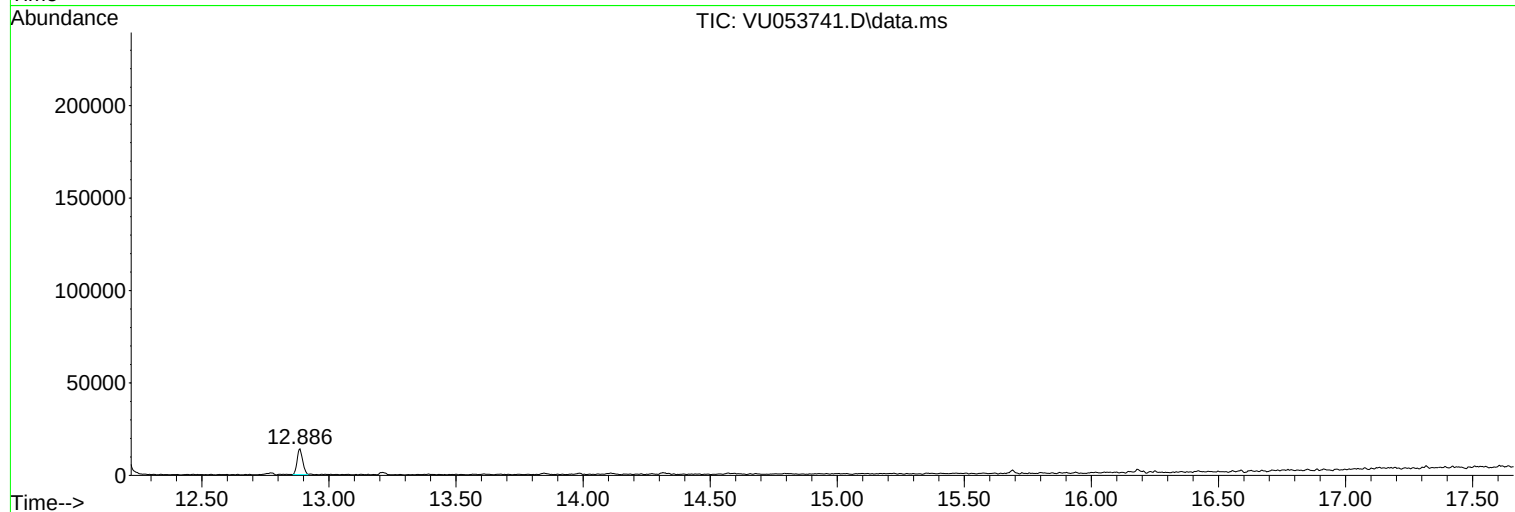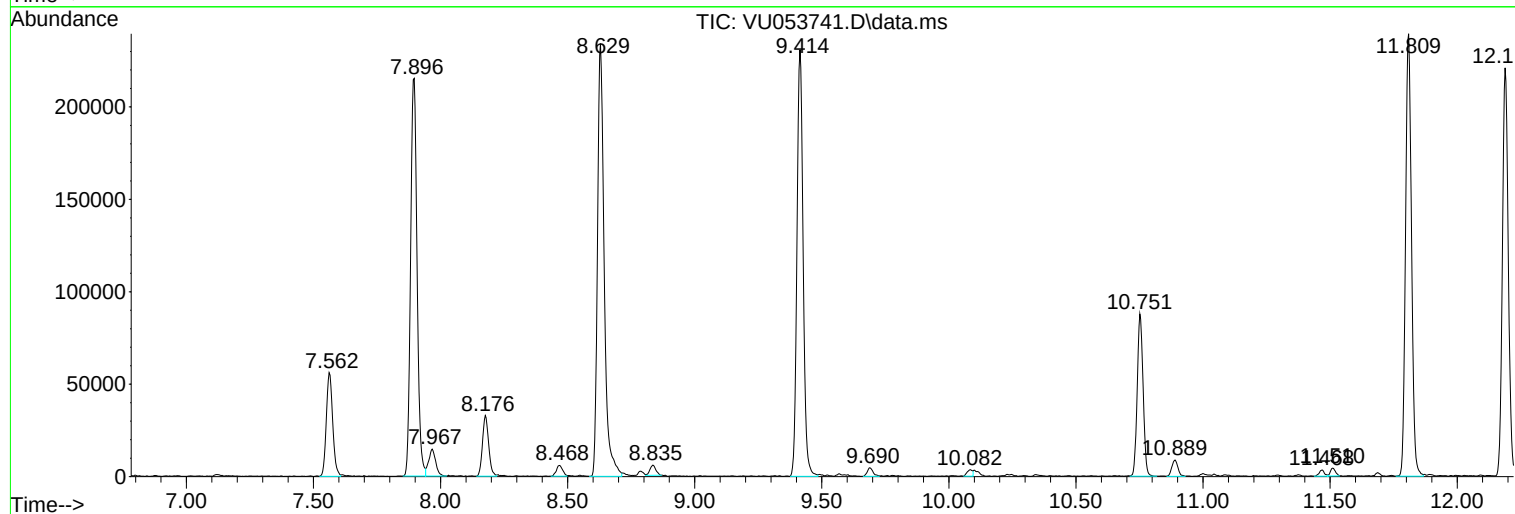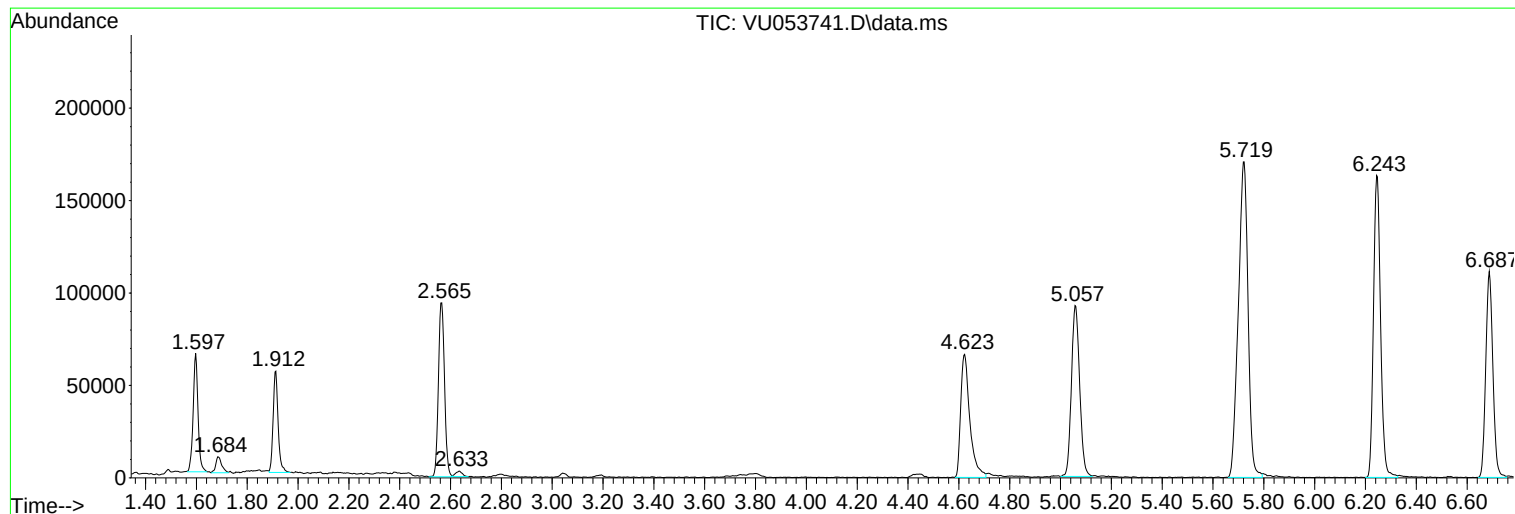

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053741.D
Acq On : 17 Apr 2023 21:00
Operator : JC/MD
Sample : 02340-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053741.D
Acq On : 17 Apr 2023 21:00
Operator : JC/MD
Sample : 02340-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------