

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
 Data File : VU053749.D
 Acq On : 18 Apr 2023 00:15
 Operator : JC/MD
 Sample : 02340-21 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	71	80	97	rVB	72229	88182	15.94%	1.906%
2	1.909	169	177	189	rBV	62713	84304	15.24%	1.822%
3	2.565	368	381	395	rBV2	115498	188662	34.10%	4.077%
4	3.041	518	529	545	rVB2	11205	20338	3.68%	0.440%
5	4.623	1009	1021	1069	rBV	86307	223473	40.39%	4.830%
6	5.057	1141	1156	1175	rVB	110004	237230	42.87%	5.127%
7	5.719	1340	1362	1383	rBV3	201953	528285	95.48%	11.417%
8	6.243	1509	1525	1541	rBV	174388	336757	60.86%	7.278%
9	6.539	1605	1617	1636	rBV	35594	66274	11.98%	1.432%
10	6.687	1649	1663	1679	rBV2	126912	250143	45.21%	5.406%
11	7.562	1919	1935	1957	rBV	63314	112161	20.27%	2.424%
12	7.893	2025	2038	2058	rBV	256454	443936	80.23%	9.594%
13	8.176	2115	2126	2147	rBV	39208	67210	12.15%	1.453%
14	8.552	2235	2243	2250	rBV6	4480	7015	1.27%	0.152%
15	8.629	2255	2267	2293	rBV	305217	553321	100.00%	11.958%
16	9.414	2498	2511	2534	rBV	242640	410263	74.15%	8.867%
17	10.751	2915	2927	2944	rVB	107116	176072	31.82%	3.805%
18	11.809	3244	3256	3275	rBV	261950	416629	75.30%	9.004%
19	12.189	3363	3374	3393	rBV	255693	416844	75.33%	9.009%




Sum of corrected areas: 4627099

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053749.D
Acq On : 18 Apr 2023 00:15
Operator : JC/MD
Sample : 02340-21 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

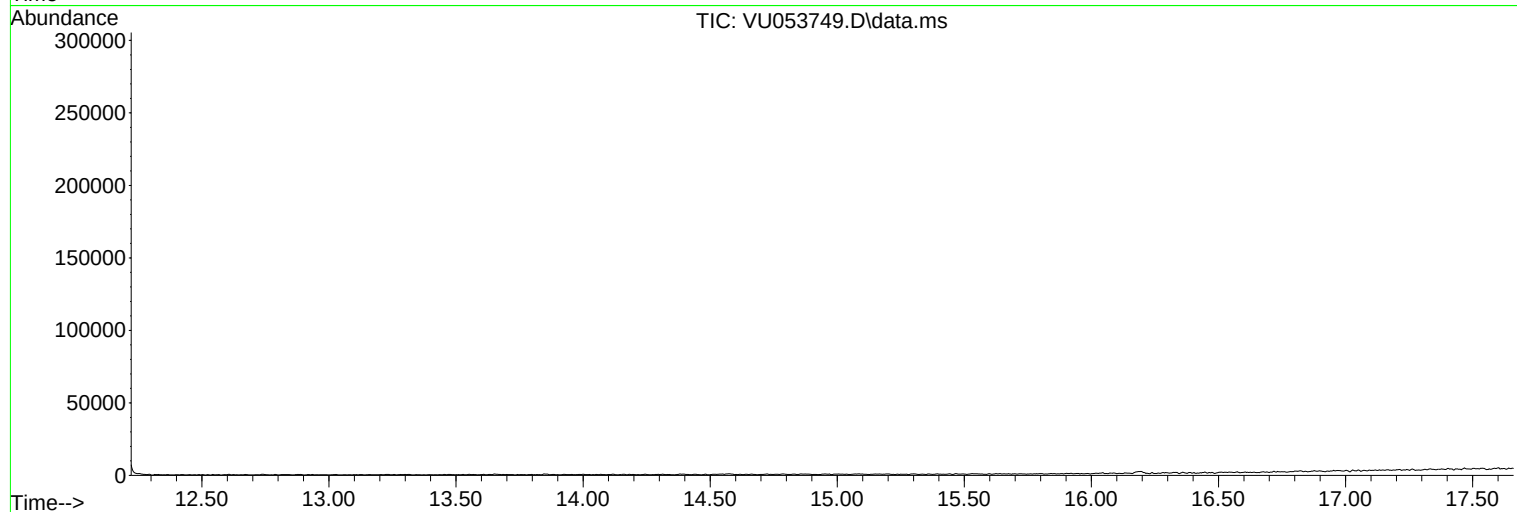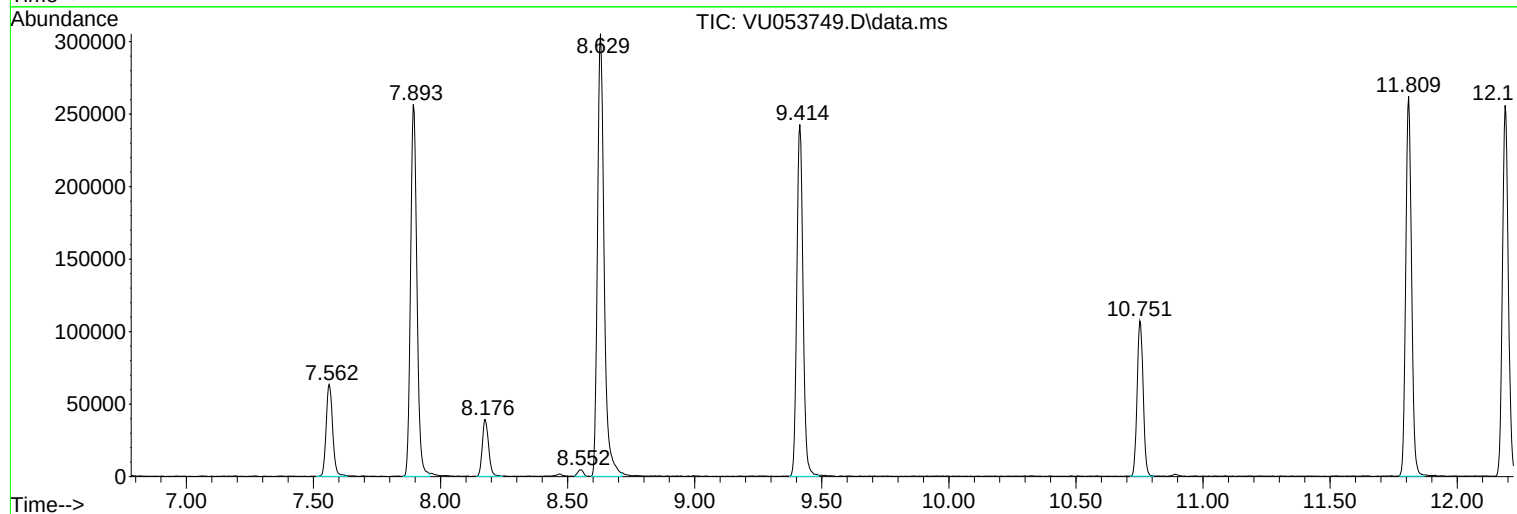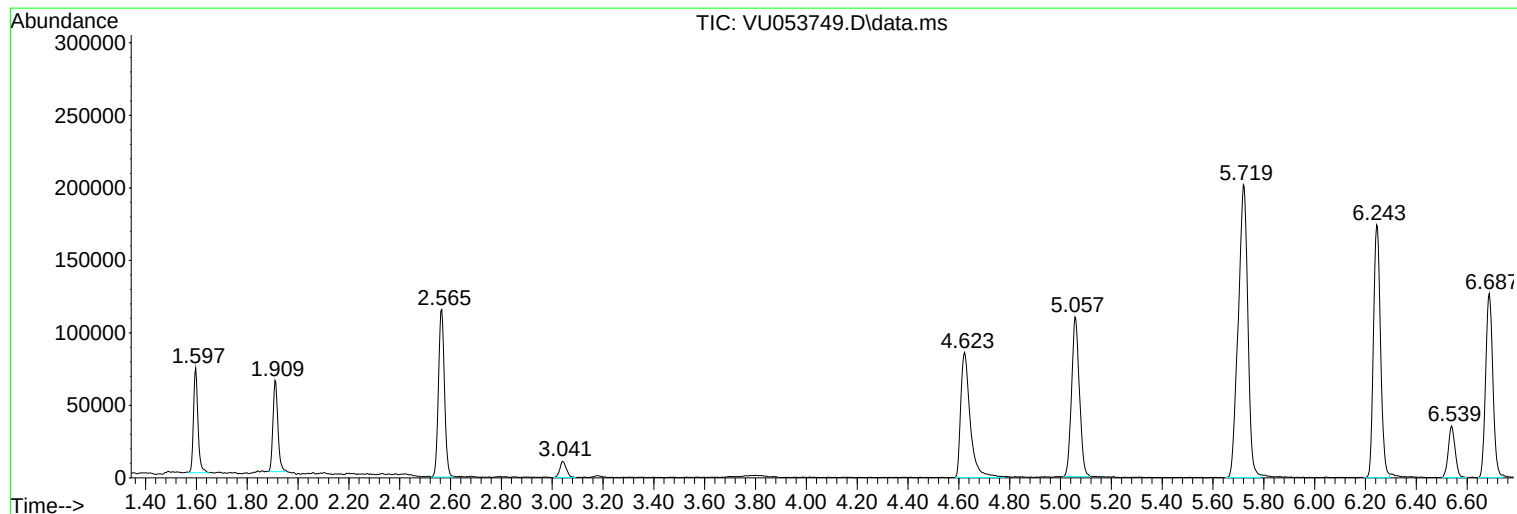

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053749.D
Acq On : 18 Apr 2023 00:15
Operator : JC/MD
Sample : 02340-21 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041723\
Data File : VU053749.D
Acq On : 18 Apr 2023 00:15
Operator : JC/MD
Sample : 02340-21 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------