

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041819\
 Data File : VU031281.D
 Acq On : 18 Apr 2019 01:33
 Operator : JC/SP
 Sample : K2410-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X49

Quant Time: Apr 18 09:41:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 18 08:39:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	226293	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	220975	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	88842	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	115651	6.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	123.80%
7) Chloroethane-d5	1.68	69	91755	5.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.60%
11) 1,1-Dichloroethene-d2	2.27	63	162347	4.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.40%
20) 2-Butanone-d5	4.20	46	261607	60.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	121.08%
24) Chloroform-d	4.64	84	146084	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
26) 1,2-Dichloroethane-d4	5.31	65	82338	5.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.80%
32) Benzene-d6	5.34	84	295844	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.33	67	99705	5.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.60%
41) Toluene-d8	7.56	98	248877	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	7.85	79	31130	4.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.80%
46) 2-Hexanone-d5	8.31	63	187058	50.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.12%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	80393	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	90147	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%


Target Compounds				Ovalue
13) Acetone	2.34	43	8668	2.458 ug/L 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041819\
Data File : VU031281.D
Acq On : 18 Apr 2019 01:33
Operator : JC/SP
Sample : K2410-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X49

Quant Time: Apr 18 09:41:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 18 08:39:25 2019
Response via : Initial Calibration

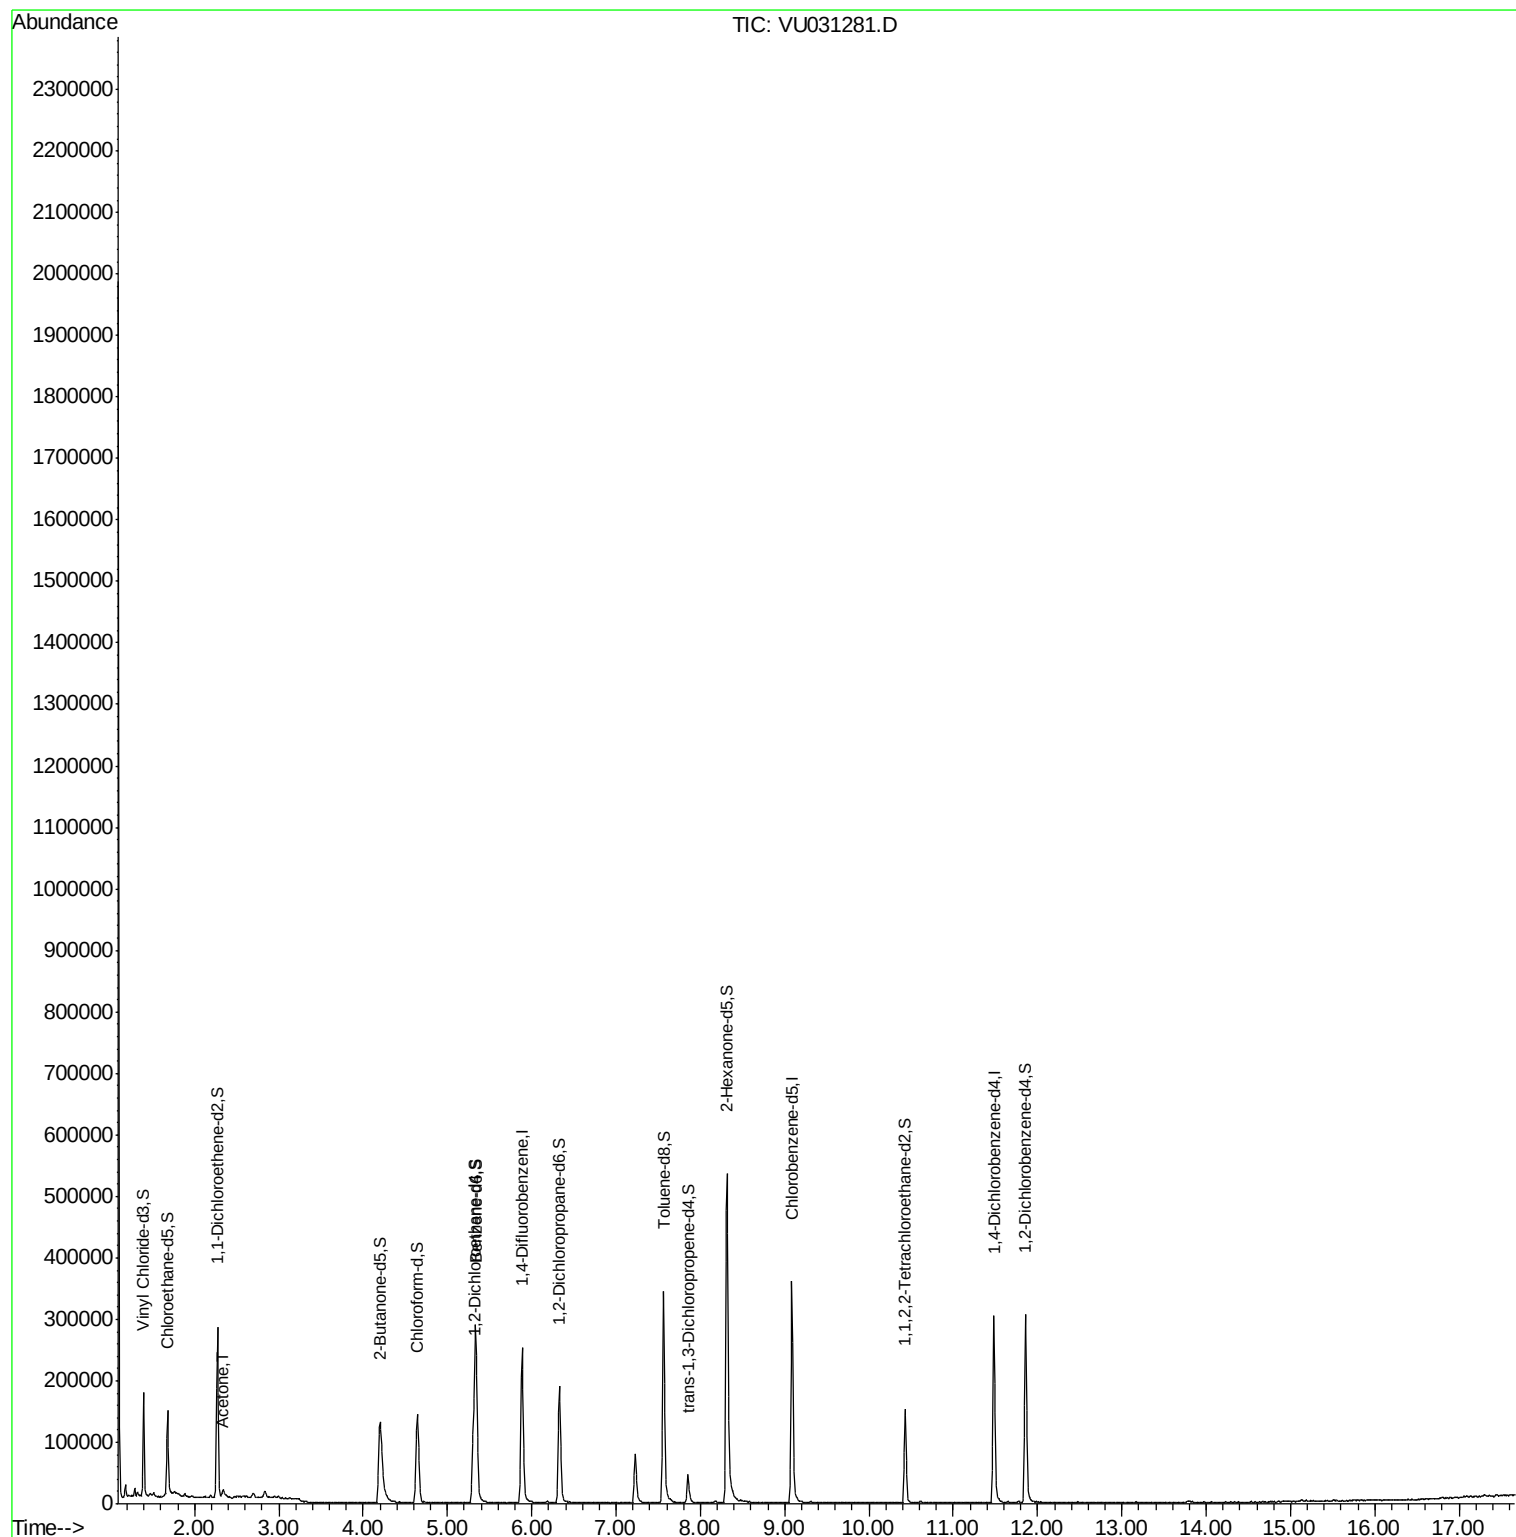

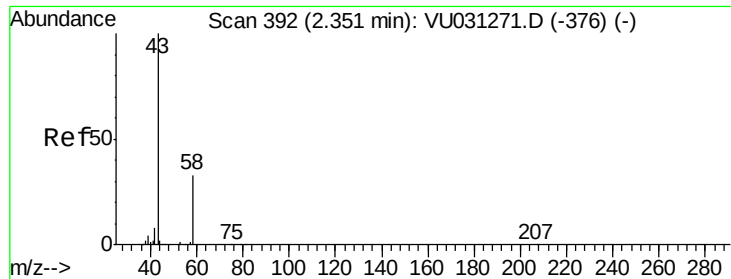

#13

Acetone

Concen: 2.458 ug/L

RT: 2.34 min Scan# 390

Delta R.T. -0.01 min

Lab File: VU031281.D

Acq: 18 Apr 2019 01:33

Instrument :

MSVOA_U

ClientSampleId :


C0X49

Tot Ion: 43 Resp: 8668

Ion Ratio Lower Upper

43 100

58 42.6 0.0 65.8

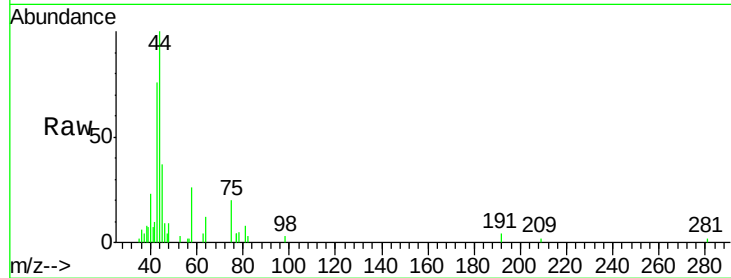

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

