

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041819\
 Data File : VU031282.D
 Acq On : 18 Apr 2019 01:57
 Operator : JC/SP
 Sample : K2410-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X51

Quant Time: Apr 18 09:43:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 18 08:39:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	236486	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	221265	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	90442	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	113208	5.80	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.00%
7) Chloroethane-d5	1.68	69	90294	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.27	63	163041	4.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.00%
20) 2-Butanone-d5	4.21	46	255997	56.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.38%
24) Chloroform-d	4.64	84	145108	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	5.31	65	80026	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.40%
32) Benzene-d6	5.34	84	292969	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.33	67	97944	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.56	98	247671	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	7.85	79	29972	3.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.60%
46) 2-Hexanone-d5	8.31	63	188664	50.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.84%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	79109	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	88692	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
13) Acetone	2.35	43	11204	3.040 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041819\
Data File : VU031282.D
Acq On : 18 Apr 2019 01:57
Operator : JC/SP
Sample : K2410-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X51

Quant Time: Apr 18 09:43:45 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 18 08:39:25 2019
Response via : Initial Calibration

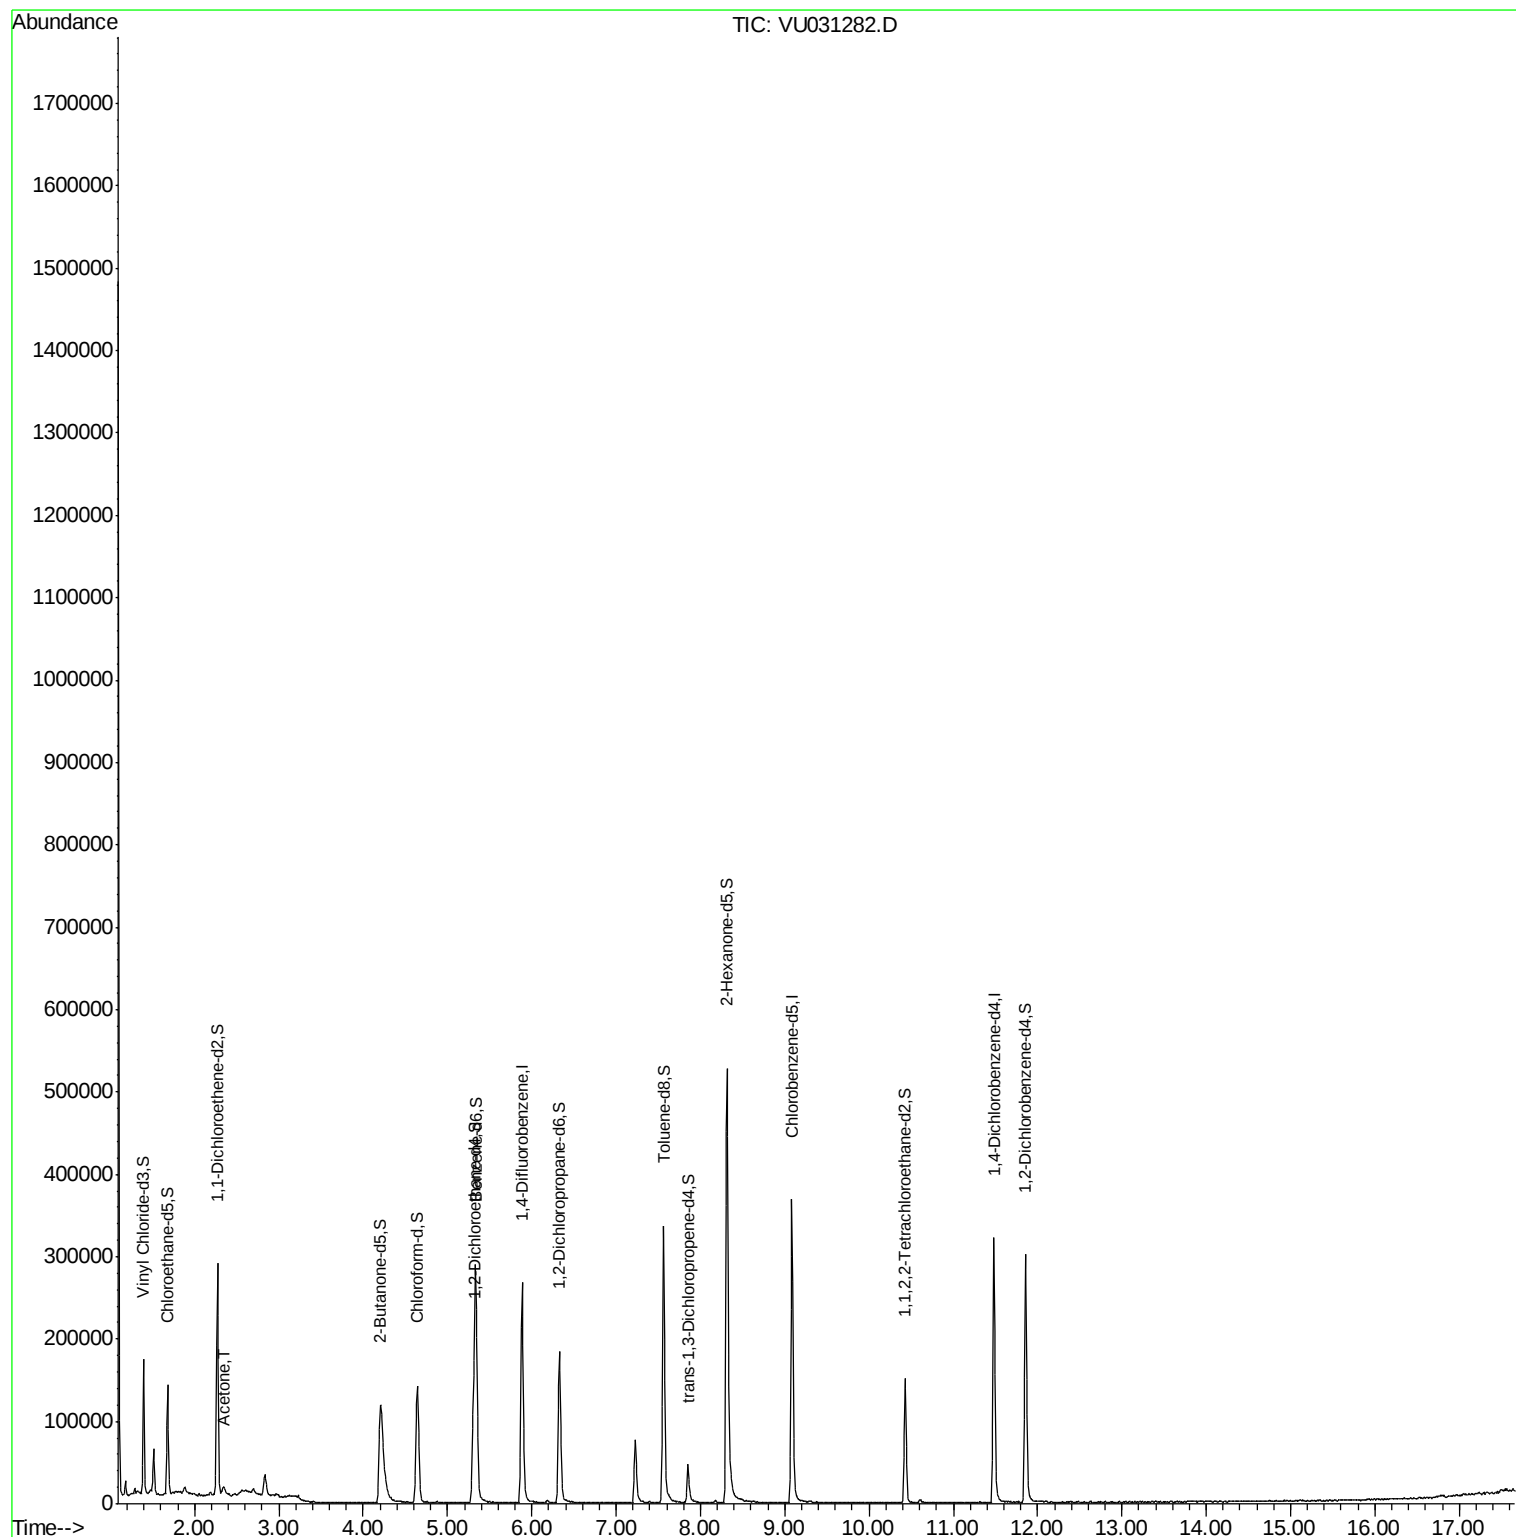

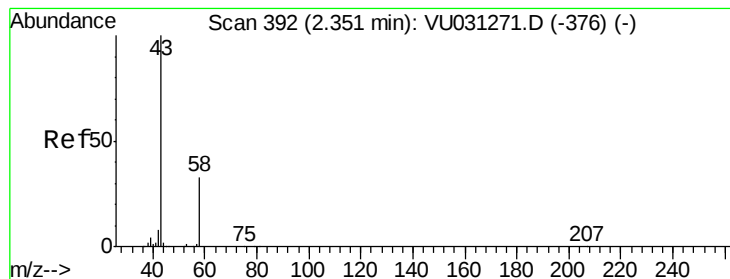

#13

Acetone

Concen: 3.040 ug/L

RT: 2.35 min Scan# 391

Delta R.T. -0.00 min

Lab File: VU031282.D

Acq: 18 Apr 2019 01:57

Instrument :

MSVOA_U

ClientSampleId :

C0X51

Tot Ion: 43 Resp: 11204

Ion Ratio Lower Upper

43 100

58 31.0 0.0 65.8

