

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041819\
 Data File : VU031293.D
 Acq On : 18 Apr 2019 06:25
 Operator : JC/SP
 Sample : K2452-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YAN04

Quant Time: Apr 27 06:44:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 18 08:39:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	209413	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	206044	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	83112	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	107266	6.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	124.20%
7) Chloroethane-d5	1.68	69	84826	5.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.40%
11) 1,1-Dichloroethene-d2	2.27	63	156871	4.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.00%
20) 2-Butanone-d5	4.20	46	233450	58.38	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.76%
24) Chloroform-d	4.64	84	140381	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.00%
26) 1,2-Dichloroethane-d4	5.31	65	79510	6.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.00%
32) Benzene-d6	5.34	84	273173	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
36) 1,2-Dichloropropane-d6	6.33	67	91238	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.56	98	231280	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	7.85	79	31712	4.47	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.40%
46) 2-Hexanone-d5	8.32	63	170682	48.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.98%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	74779	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	91072	5.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.00%


Target Compounds					Ovalue
13) Acetone	2.34	43	31702	9.715 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041819\
Data File : VU031293.D
Acq On : 18 Apr 2019 06:25
Operator : JC/SP
Sample : K2452-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YAN04

Quant Time: Apr 27 06:44:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 18 08:39:25 2019
Response via : Initial Calibration

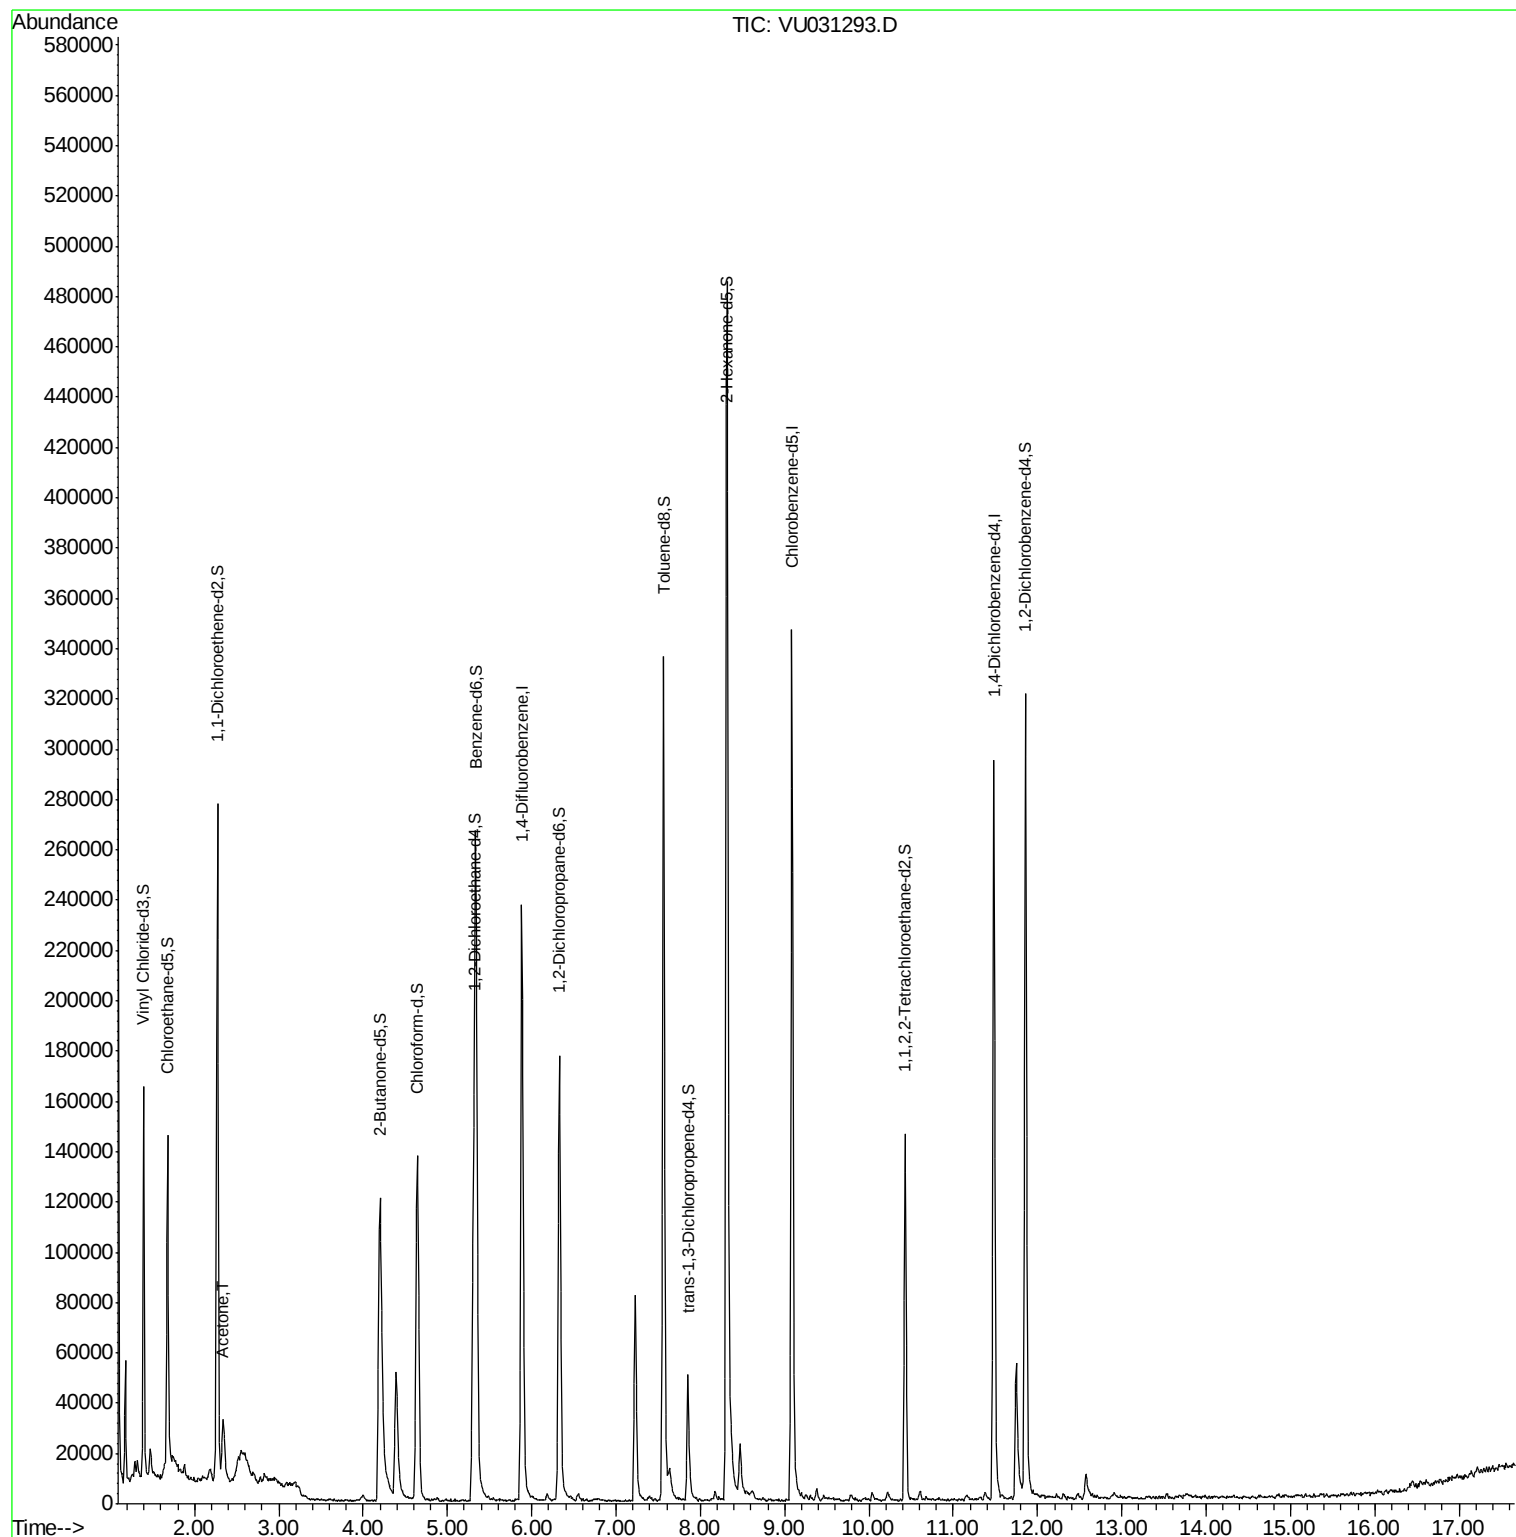

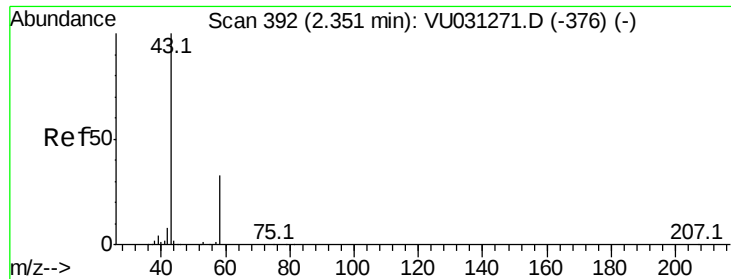

#13

Acetone

Concen: 9.715 ug/L

RT: 2.34 min Scan# 388

Delta R.T. -0.01 min

Lab File: VU031293.D

Acq: 18 Apr 2019 06:25

Instrument :
MSVOA_U
ClientSampleId :
YAN04

Tot Ion: 43 Resp: 31702

Ion Ratio Lower Upper

43 100

58 30.5 0.0 65.8

