


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041819\
Data File : VU031264.D
Acq On : 17 Apr 2019 17:18
Operator : JC/SP
Sample : BFB40
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041819WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 18 08:52:58 2019

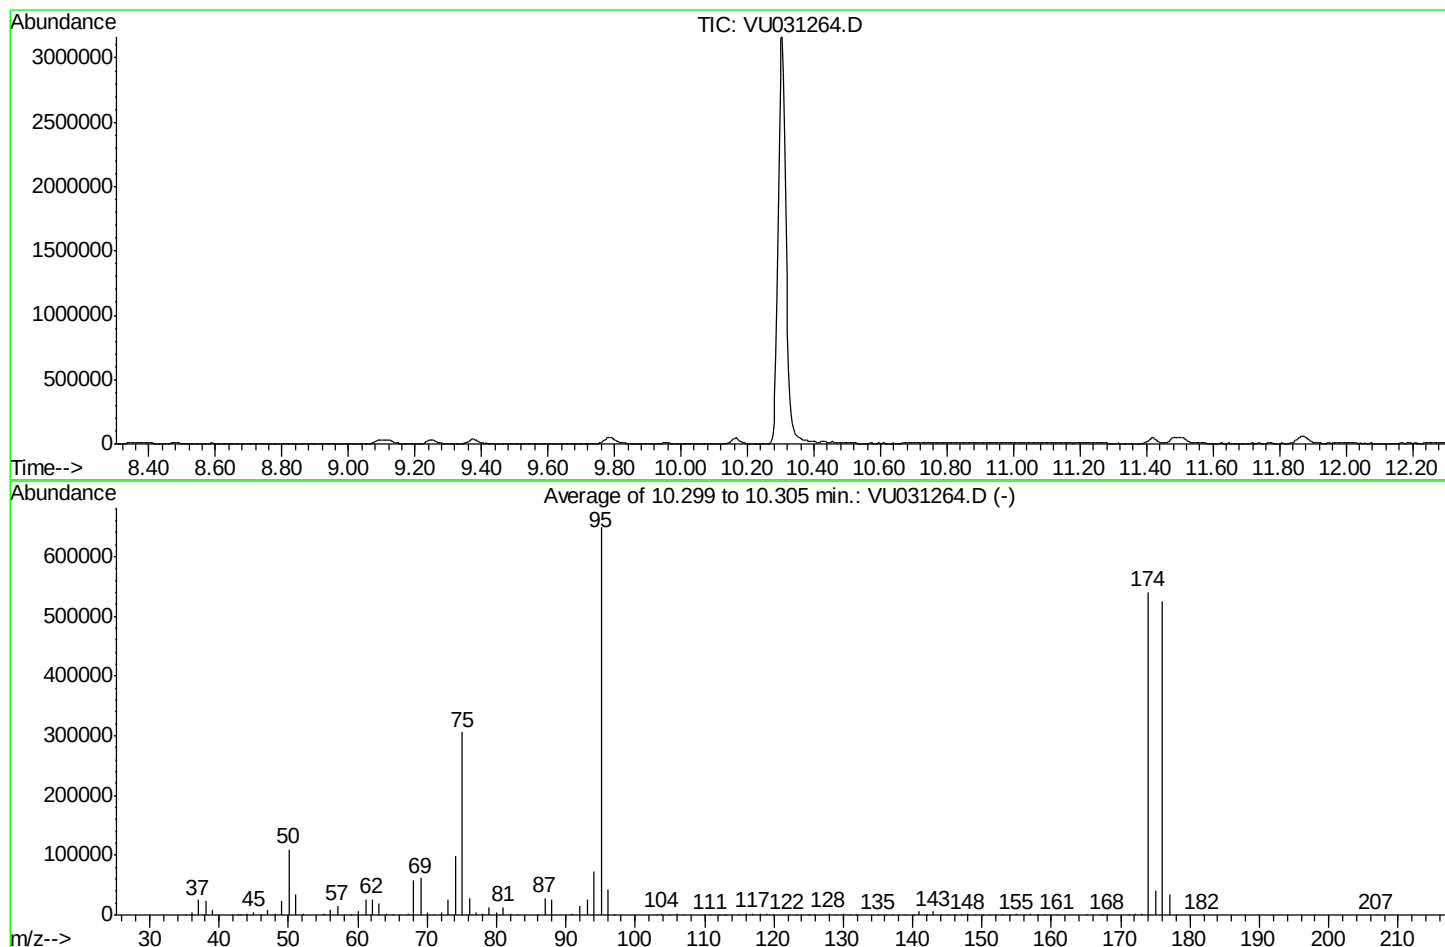

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	109917	PASS
75	95	30	80	47.1	306005	PASS
95	95	100	100	100.0	649173	PASS
96	95	5	9	6.5	42416	PASS
173	174	0.00	2	0.4	2185	PASS
174	95	50	120	83.3	540970	PASS
175	174	5	9	7.5	40368	PASS
176	174	95	101	97.2	525824	PASS
177	176	5	9	6.5	34162	PASS

Scan 2850 (10.254 min): VU031264.D
BFB40

m/z	Abundance
36.00	110.0
39.20	115.0
40.00	960.0
43.90	792.0
165.20	277.0
166.00	210.0
167.10	250.0
168.20	152.0
169.20	109.0
184.30	160.0
206.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.10	4442.0
37.00	24008.0
38.10	21440.0
39.00	9148.0
40.10	774.0
42.60	118.0
44.10	3469.0
45.00	4491.0
46.10	356.0
47.00	8624.0
48.00	2822.0
49.00	22944.0
50.00	104880.0
51.10	33664.0
52.10	1440.0
55.00	1160.0
56.00	7346.0
57.10	14127.0
58.10	777.0
59.00	216.0
60.10	5056.0
61.10	24424.0
62.10	25744.0
63.10	17288.0
64.00	1957.0
65.10	1010.0
66.00	145.0
67.20	1831.0
68.00	55944.0
69.10	58280.0
70.00	4693.0
71.00	193.0
72.20	3036.0
73.00	25048.0
74.10	94000.0
75.10	289600.0
76.10	25760.0
77.00	4174.0
78.10	2160.0
78.90	12947.0
80.00	3443.0
81.00	13366.0
82.00	2426.0
83.10	266.0
86.00	969.0
87.00	26272.0
88.00	25280.0
90.90	2005.0
92.10	14290.0
93.10	22848.0
94.10	67216.0
95.10	608960.0
96.10	40496.0
97.10	1194.0
103.00	266.0
103.90	2492.0
105.00	916.0
106.00	1859.0
106.90	556.0
110.00	147.0
110.90	272.0
112.10	180.0
112.80	405.0
114.90	656.0
116.00	1688.0
116.90	2926.0
118.00	1904.0
119.00	2487.0
119.80	100.0
122.10	113.0
123.20	245.0
123.90	338.0
125.00	214.0
128.00	2234.0
128.90	963.0
129.90	1955.0
131.00	724.0
131.80	268.0
135.00	1051.0
136.00	135.0
137.00	1044.0
138.90	285.0
140.10	459.0
141.00	5579.0
142.00	721.0
143.00	5556.0
144.10	349.0
145.00	810.0
146.00	1131.0
146.90	432.0
148.00	1354.0
149.00	356.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

150.10	607.0
152.00	359.0
152.90	410.0
154.00	595.0
155.00	1607.0
156.10	132.0
157.00	1216.0
157.80	102.0
159.00	707.0
160.90	512.0
165.10	341.0
166.10	162.0
167.20	339.0
168.00	324.0
171.00	306.0
172.10	1565.0
173.10	6555.0
174.00	491264.0
175.00	36608.0
176.00	477248.0
177.00	31528.0
178.00	887.0
207.10	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
35.20	132.0
36.10	5037.0
37.00	25784.0
38.10	23536.0
39.10	9356.0
40.10	824.0
42.70	128.0
44.00	3721.0
45.00	4632.0
46.10	379.0
47.10	8997.0
48.00	3165.0
49.00	24968.0
50.00	113952.0
51.10	35904.0
52.10	1579.0
55.00	1318.0
56.00	7988.0
57.10	15830.0
58.00	846.0
59.00	258.0
60.00	5969.0
61.10	27104.0
62.10	27480.0
63.10	19600.0
64.00	2124.0
65.10	981.0
66.00	164.0
68.00	60840.0
69.10	63600.0
70.00	4910.0
71.00	198.0
72.10	3481.0
73.00	27056.0
74.10	101976.0
75.10	316224.0
76.10	27976.0
77.00	4243.0
78.00	2259.0
78.90	13797.0
80.00	3865.0
81.00	14399.0
82.00	2591.0
83.10	289.0
86.00	1063.0
87.00	29872.0
88.00	27304.0
90.90	2287.0
92.10	16052.0
93.10	25976.0
94.10	74560.0
95.10	671104.0
96.10	43560.0
97.00	1147.0
103.00	175.0
103.90	2720.0
104.90	1044.0
106.00	2012.0
106.90	618.0
110.00	252.0
110.90	282.0
112.10	240.0
113.00	451.0
115.00	749.0
116.00	1724.0
117.00	3222.0
118.00	2072.0
119.00	3079.0
119.90	136.0
122.00	165.0
123.10	233.0
123.90	324.0
125.10	253.0
127.90	2533.0
128.90	1004.0
130.00	2195.0
131.00	900.0
131.80	306.0
135.00	1105.0
136.00	208.0
137.10	1023.0
139.00	315.0
140.20	574.0
141.00	6282.0
142.00	767.0
143.00	6389.0
144.10	316.0
145.00	789.0
146.00	1169.0
146.90	419.0
148.00	1521.0
149.10	376.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

150.00	767.0
151.00	130.0
152.00	412.0
152.90	503.0
154.00	686.0
155.00	1757.0
156.10	114.0
156.90	1164.0
158.10	162.0
159.00	756.0
160.90	478.0
165.10	346.0
166.10	163.0
167.10	238.0
168.00	262.0
169.00	111.0
171.10	404.0
172.10	1618.0
174.00	558400.0
175.00	41792.0
176.00	543488.0
177.00	35432.0
178.00	958.0
184.10	124.0
207.10	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.10	4897.0
37.00	25456.0
38.00	23504.0
39.10	9143.0
40.10	937.0
43.10	190.0
44.00	3696.0
45.00	4313.0
46.10	345.0
47.10	9038.0
48.00	3365.0
49.10	24184.0
50.10	110920.0
51.10	34488.0
52.10	1521.0
55.00	1593.0
56.10	7756.0
57.10	15312.0
58.00	804.0
59.10	196.0
60.00	6082.0
61.10	26992.0
62.10	27192.0
63.10	19960.0
64.10	2060.0
65.00	783.0
65.90	131.0
67.20	1828.0
68.00	59776.0
69.10	63272.0
70.10	4672.0
71.00	162.0
72.10	3508.0
73.10	26456.0
74.10	100416.0
75.10	312192.0
76.10	27784.0
77.00	3858.0
78.00	2229.0
79.00	13676.0
80.00	4051.0
81.00	13930.0
82.00	2637.0
83.00	358.0
86.00	971.0
87.00	30088.0
88.00	26736.0
90.90	2230.0
92.00	16536.0
93.10	26608.0
94.10	74888.0
95.10	667456.0
96.10	43192.0
97.00	1080.0
103.90	2522.0
104.90	1049.0
106.00	2021.0
106.90	553.0
109.90	390.0
110.80	299.0
112.00	266.0
113.00	534.0
115.00	815.0
116.00	1788.0
117.00	3280.0
117.90	1992.0
119.00	3144.0
119.90	155.0
122.00	202.0
123.10	168.0
123.90	321.0
125.10	269.0
125.80	151.0
127.90	2621.0
128.90	992.0
130.00	2283.0
131.00	991.0
131.80	215.0
135.10	1031.0
136.10	233.0
137.00	991.0
138.90	298.0
140.20	576.0
141.00	6323.0
142.00	732.0
143.00	6577.0
144.10	267.0
145.00	686.0
146.00	1088.0
147.00	379.0
148.00	1512.0
149.00	367.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

150.00	766.0
151.00	170.0
152.00	395.0
152.90	475.0
154.00	604.0
155.00	1848.0
156.90	1077.0
158.10	186.0
159.00	759.0
160.90	398.0
165.00	362.0
166.20	158.0
167.00	230.0
167.40	190.0
168.00	339.0
169.00	128.0
171.20	393.0
172.00	1444.0
174.00	573248.0
175.00	42704.0
176.00	556736.0
177.00	35528.0
178.00	990.0
181.80	124.0
184.10	193.0
207.00	218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40