

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041823\
 Data File : VU053760.D
 Acq On : 18 Apr 2023 15:25
 Operator : JC/MD
 Sample : 02340-20 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	55732	67311	10.57%	1.384%
2	1.912	169	178	196	rVB	50389	71201	11.18%	1.464%
3	2.575	367	384	399	rBV4	218866	416545	65.41%	8.565%
4	3.041	520	529	545	rVB3	7529	13910	2.18%	0.286%
5	3.864	772	785	810	rVB	43398	104105	16.35%	2.141%
6	4.623	1005	1021	1053	rBV	61917	186527	29.29%	3.836%
7	5.057	1141	1156	1174	rBV	88856	195380	30.68%	4.018%
8	5.722	1343	1363	1384	rBV2	164758	430798	67.64%	8.859%
9	6.247	1509	1526	1541	rBV	166457	314835	49.43%	6.474%
10	6.539	1602	1617	1642	rBV	335971	636870	100.00%	13.096%
11	6.687	1650	1663	1688	rVB2	106548	206975	32.50%	4.256%
12	7.562	1923	1935	1957	rBV	52699	93493	14.68%	1.922%
13	7.893	2023	2038	2058	rBV	203479	359018	56.37%	7.382%
14	8.176	2114	2126	2140	rBV	31652	52669	8.27%	1.083%
15	8.549	2232	2242	2256	rBV2	43807	74100	11.64%	1.524%
16	8.629	2256	2267	2299	rBV	211282	402822	63.25%	8.283%
17	9.414	2499	2511	2536	rBV	230281	383629	60.24%	7.889%
18	10.751	2916	2927	2942	rBV2	83821	135171	21.22%	2.780%
19	11.809	3244	3256	3272	rBV	237781	379241	59.55%	7.798%
20	12.188	3362	3374	3393	rBV	206860	338500	53.15%	6.961%




Sum of corrected areas: 4863100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041823\
Data File : VU053760.D
Acq On : 18 Apr 2023 15:25
Operator : JC/MD
Sample : 02340-20 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

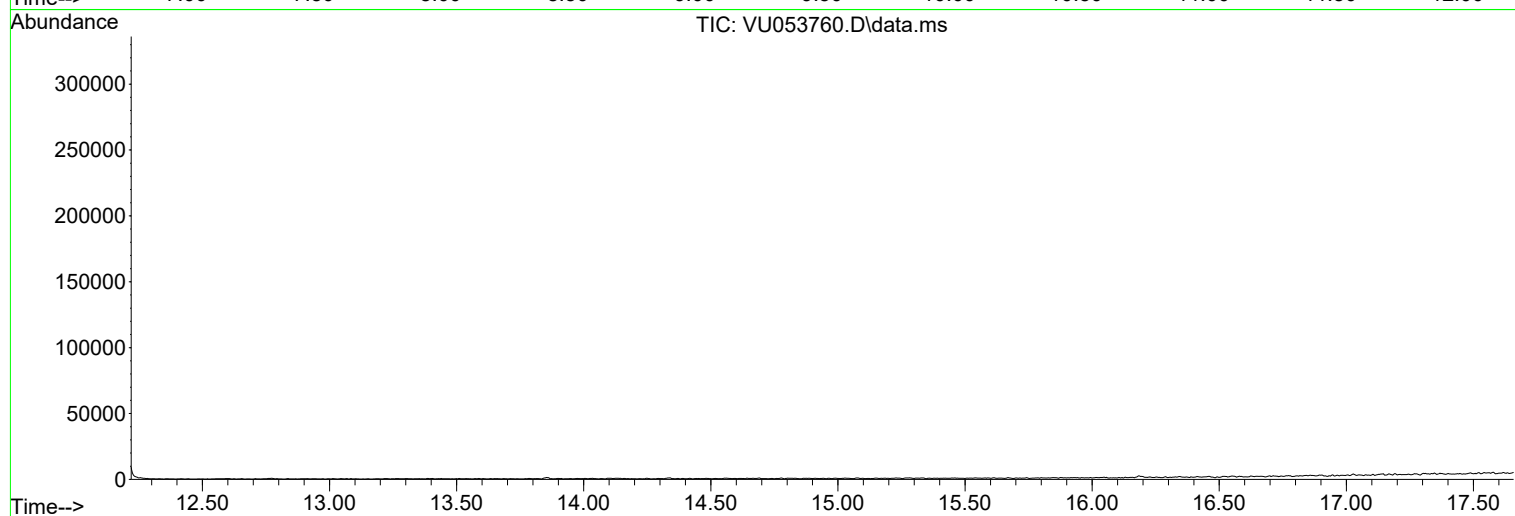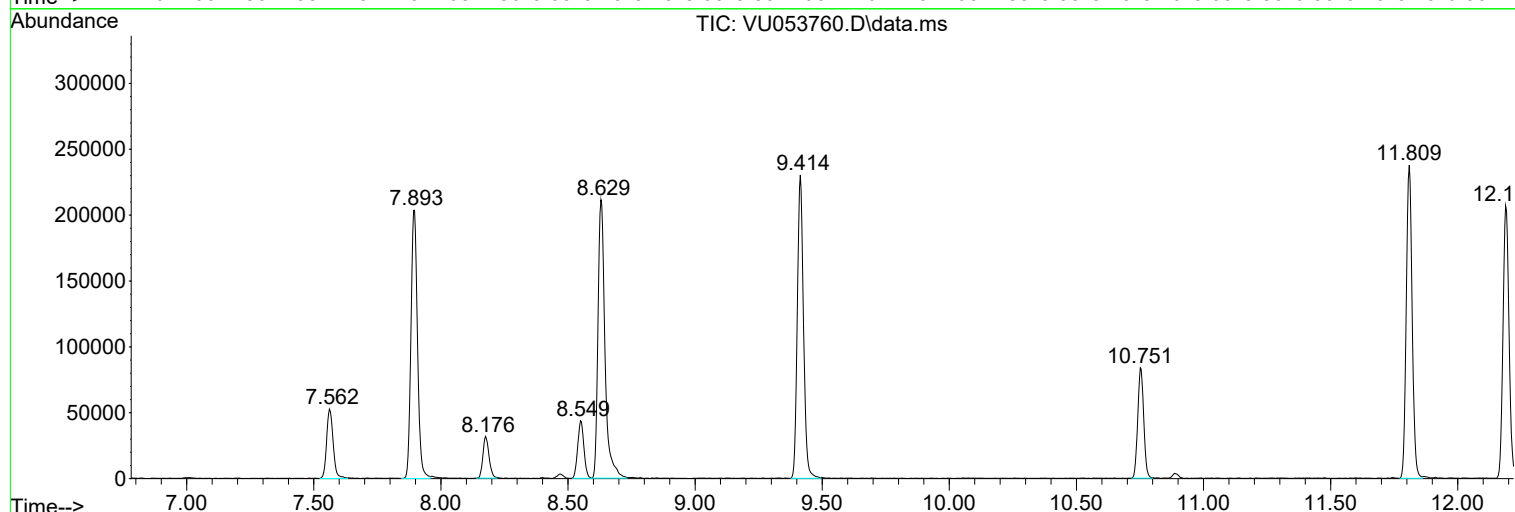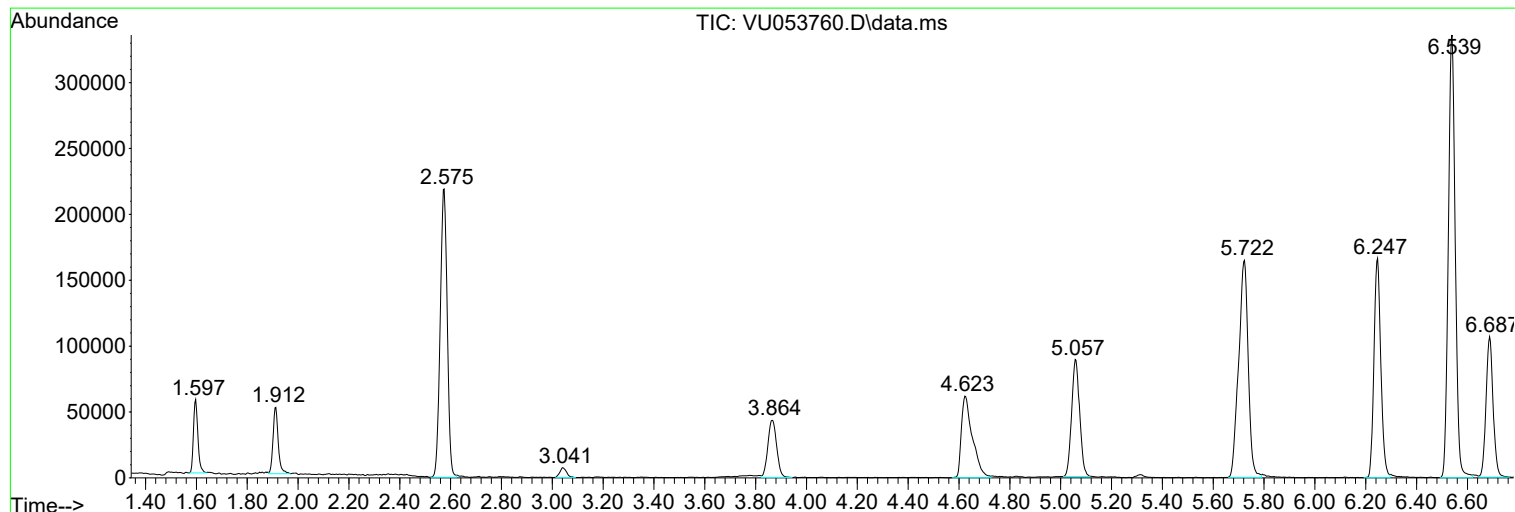

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041823\
Data File : VU053760.D
Acq On : 18 Apr 2023 15:25
Operator : JC/MD
Sample : 02340-20 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041823\
Data File : VU053760.D
Acq On : 18 Apr 2023 15:25
Operator : JC/MD
Sample : 02340-20 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc