
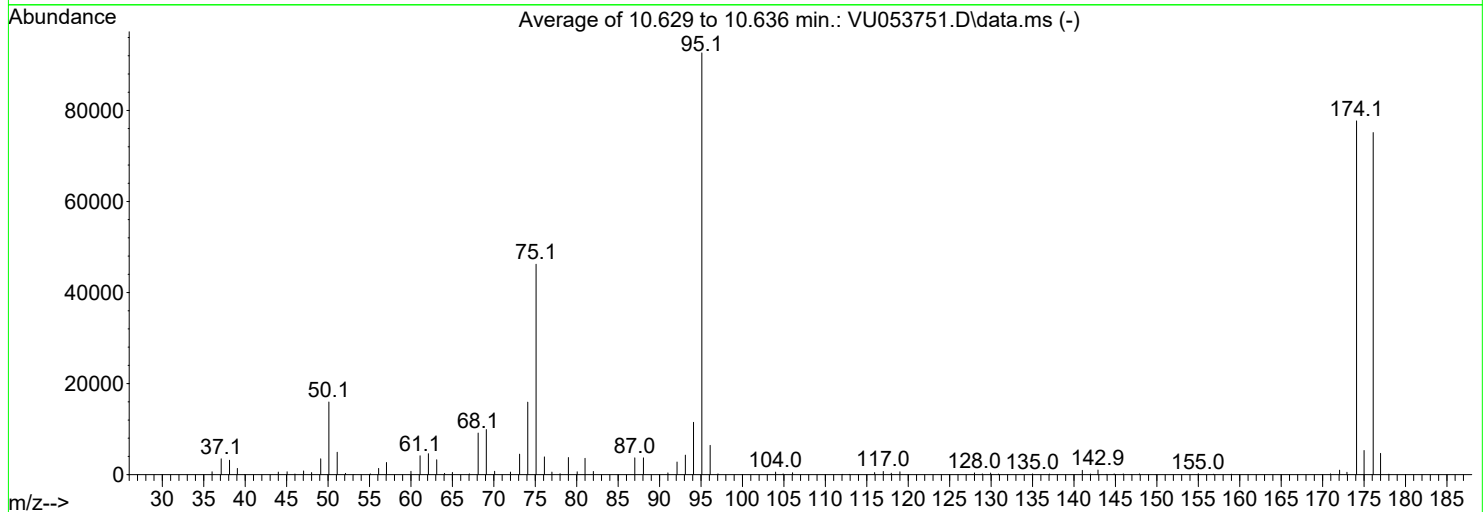


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041823\
Data File : VU053751.D
Acq On : 18 Apr 2023 08:58
Operator : JC/MD
Sample : BFB005
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB005

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 19 04:58:28 2023

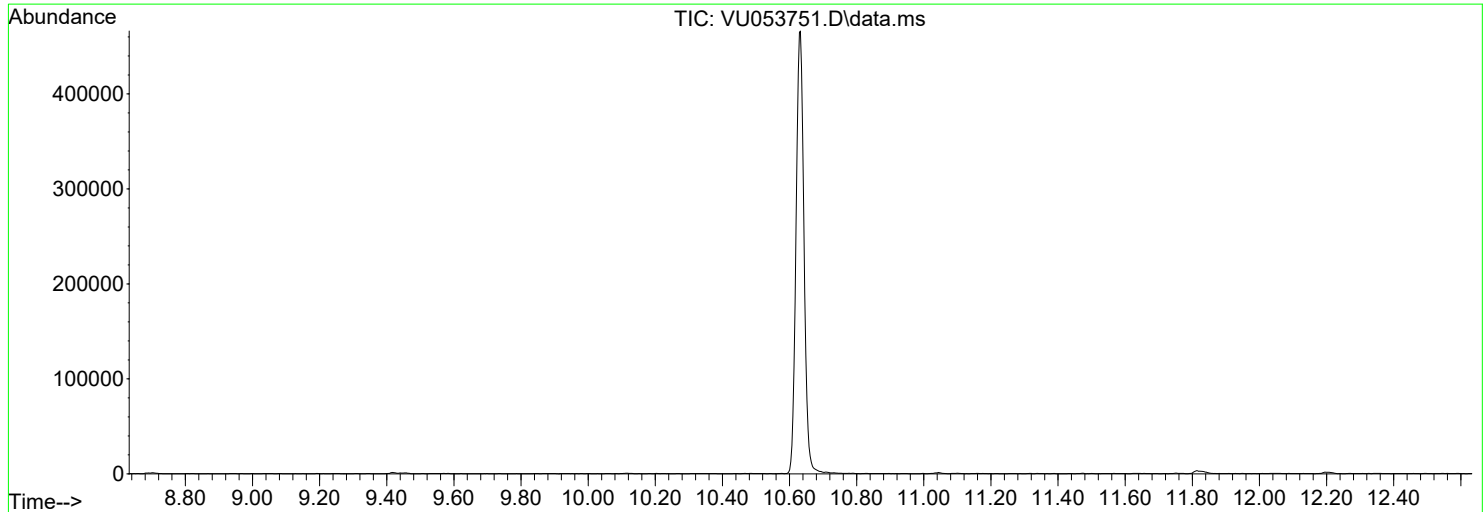

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	15948	PASS
75	95	30	80	49.9	46200	PASS
95	95	100	100	100.0	92643	PASS
96	95	5	9	6.9	6427	PASS
173	174	0.00	2	0.7	520	PASS
174	95	50	120	83.9	77701	PASS
175	174	5	9	6.9	5326	PASS
176	174	95	101	96.7	75136	PASS
177	176	5	9	6.2	4670	PASS

m/z	Abundance
44.10	251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
36.00	660.0
37.10	3355.0
38.10	3395.0
39.10	1454.0
44.00	837.0
45.00	657.0
46.00	104.0
47.00	910.0
48.00	418.0
49.10	3555.0
50.10	16792.0
51.10	5156.0
52.10	355.0
55.10	211.0
56.10	1476.0
57.10	2828.0
60.00	810.0
61.10	4266.0
62.10	4748.0
63.10	3434.0
64.10	332.0
65.00	486.0
67.00	223.0
68.10	9663.0
69.10	10622.0
70.10	802.0
72.00	530.0
73.10	4622.0
74.10	16528.0
75.10	47592.0
76.10	4071.0
77.00	590.0
78.10	168.0
79.00	3814.0
80.00	671.0
81.00	3775.0
82.00	738.0
87.00	3677.0
88.10	3772.0
91.00	433.0
92.10	2755.0
93.10	4313.0
94.10	11999.0
95.10	95488.0
96.10	6670.0
97.10	191.0
104.00	541.0
105.00	187.0
106.00	406.0
112.10	105.0
112.90	134.0
115.90	492.0
117.00	756.0
118.00	329.0
119.00	690.0
128.00	413.0
129.00	133.0
129.90	317.0
130.90	126.0
135.00	190.0
137.00	159.0
141.00	969.0
142.10	118.0
142.90	940.0
143.90	130.0
144.80	175.0
146.00	182.0
146.90	108.0
147.90	160.0
155.00	228.0
156.90	118.0
159.00	118.0
170.90	150.0
172.00	982.0
172.90	544.0
174.10	79016.0
175.00	5529.0
176.10	75456.0
177.00	4800.0
178.00	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
36.00	632.0
37.10	3586.0
38.10	3243.0
39.00	1393.0
44.00	847.0
45.10	655.0
46.00	144.0
47.00	806.0
48.00	452.0
49.10	3596.0
50.10	16488.0
51.10	5054.0
52.10	315.0
55.10	199.0
56.10	1431.0
57.00	2748.0
60.00	755.0
61.10	4237.0
62.10	4762.0
63.10	3344.0
64.00	267.0
65.00	497.0
67.00	184.0
68.10	9568.0
69.10	10123.0
70.10	753.0
72.00	583.0
73.10	4641.0
74.10	16552.0
75.10	47544.0
76.10	3966.0
77.00	571.0
78.10	215.0
79.00	3890.0
80.00	612.0
81.00	3731.0
82.00	701.0
87.00	3697.0
88.00	3761.0
91.00	369.0
92.10	2880.0
93.10	4481.0
94.10	11906.0
95.10	95664.0
96.10	6641.0
97.00	172.0
104.00	583.0
104.90	189.0
106.00	470.0
112.00	100.0
112.90	108.0
116.00	482.0
117.00	735.0
118.00	315.0
119.00	658.0
128.00	394.0
128.90	162.0
130.00	347.0
130.90	157.0
135.00	196.0
137.00	147.0
141.00	964.0
142.00	155.0
142.90	1063.0
143.90	128.0
144.80	191.0
145.90	189.0
147.90	159.0
155.00	241.0
156.90	100.0
159.00	131.0
170.90	178.0
172.10	1034.0
172.90	533.0
174.10	80032.0
175.00	5484.0
176.10	77096.0
177.00	4714.0
178.00	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
36.00	576.0
37.10	3461.0
38.10	2911.0
39.00	1311.0
39.90	110.0
44.00	743.0
45.10	635.0
46.00	139.0
47.10	685.0
48.00	480.0
49.10	3317.0
50.10	14563.0
51.10	4551.0
52.10	211.0
53.10	113.0
55.10	154.0
56.10	1257.0
57.00	2489.0
60.00	662.0
61.10	3941.0
62.10	4347.0
63.10	2979.0
64.00	234.0
65.00	466.0
67.10	159.0
68.10	8194.0
69.10	9008.0
70.10	659.0
72.00	534.0
73.10	4189.0
74.10	14656.0
75.10	43464.0
76.10	3646.0
77.00	509.0
77.90	255.0
79.00	3594.0
80.10	603.0
81.00	3301.0
82.00	652.0
87.00	3711.0
88.00	3511.0
91.00	315.0
92.10	2681.0
93.10	4060.0
94.10	10629.0
95.10	86776.0
96.10	5971.0
97.00	171.0
104.00	545.0
104.80	161.0
106.10	452.0
116.00	421.0
117.00	678.0
117.80	338.0
119.00	525.0
128.00	371.0
128.90	214.0
130.00	369.0
130.90	153.0
135.00	169.0
137.10	143.0
141.00	939.0
141.90	168.0
142.90	1022.0
144.90	165.0
145.90	185.0
147.90	169.0
149.90	112.0
155.00	205.0
156.80	111.0
159.00	109.0
171.00	158.0
172.10	981.0
173.00	483.0
174.10	74056.0
175.00	4964.0
176.10	72856.0
177.00	4496.0
178.00	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005