

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041919\
 Data File : VU031306.D
 Acq On : 18 Apr 2019 14:52
 Operator : JC/SP
 Sample : K2410-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XE3

Quant Time: Apr 19 04:52:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 19 04:38:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	199474	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	196329	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	77858	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	105687	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.68	69	83679	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.27	63	156819	3.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.20%
20) 2-Butanone-d5	4.20	46	215076	50.03	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.06%
24) Chloroform-d	4.64	84	137130	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.31	65	76743	5.05	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.00%
32) Benzene-d6	5.34	84	263268	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.33	67	85707	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.56	98	269378	5.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.20%
43) trans-1,3-Dichloropropene-	7.85	79	40153	5.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	116.60%
46) 2-Hexanone-d5	8.31	63	157304	49.40	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.80%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	71378	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	81338	5.36	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.20%


Target Compounds					Ovalue
13) Acetone	2.34	43	14711	3.076 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041919\
Data File : VU031306.D
Acq On : 18 Apr 2019 14:52
Operator : JC/SP
Sample : K2410-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XE3

Quant Time: Apr 19 04:52:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 19 04:38:37 2019
Response via : Initial Calibration

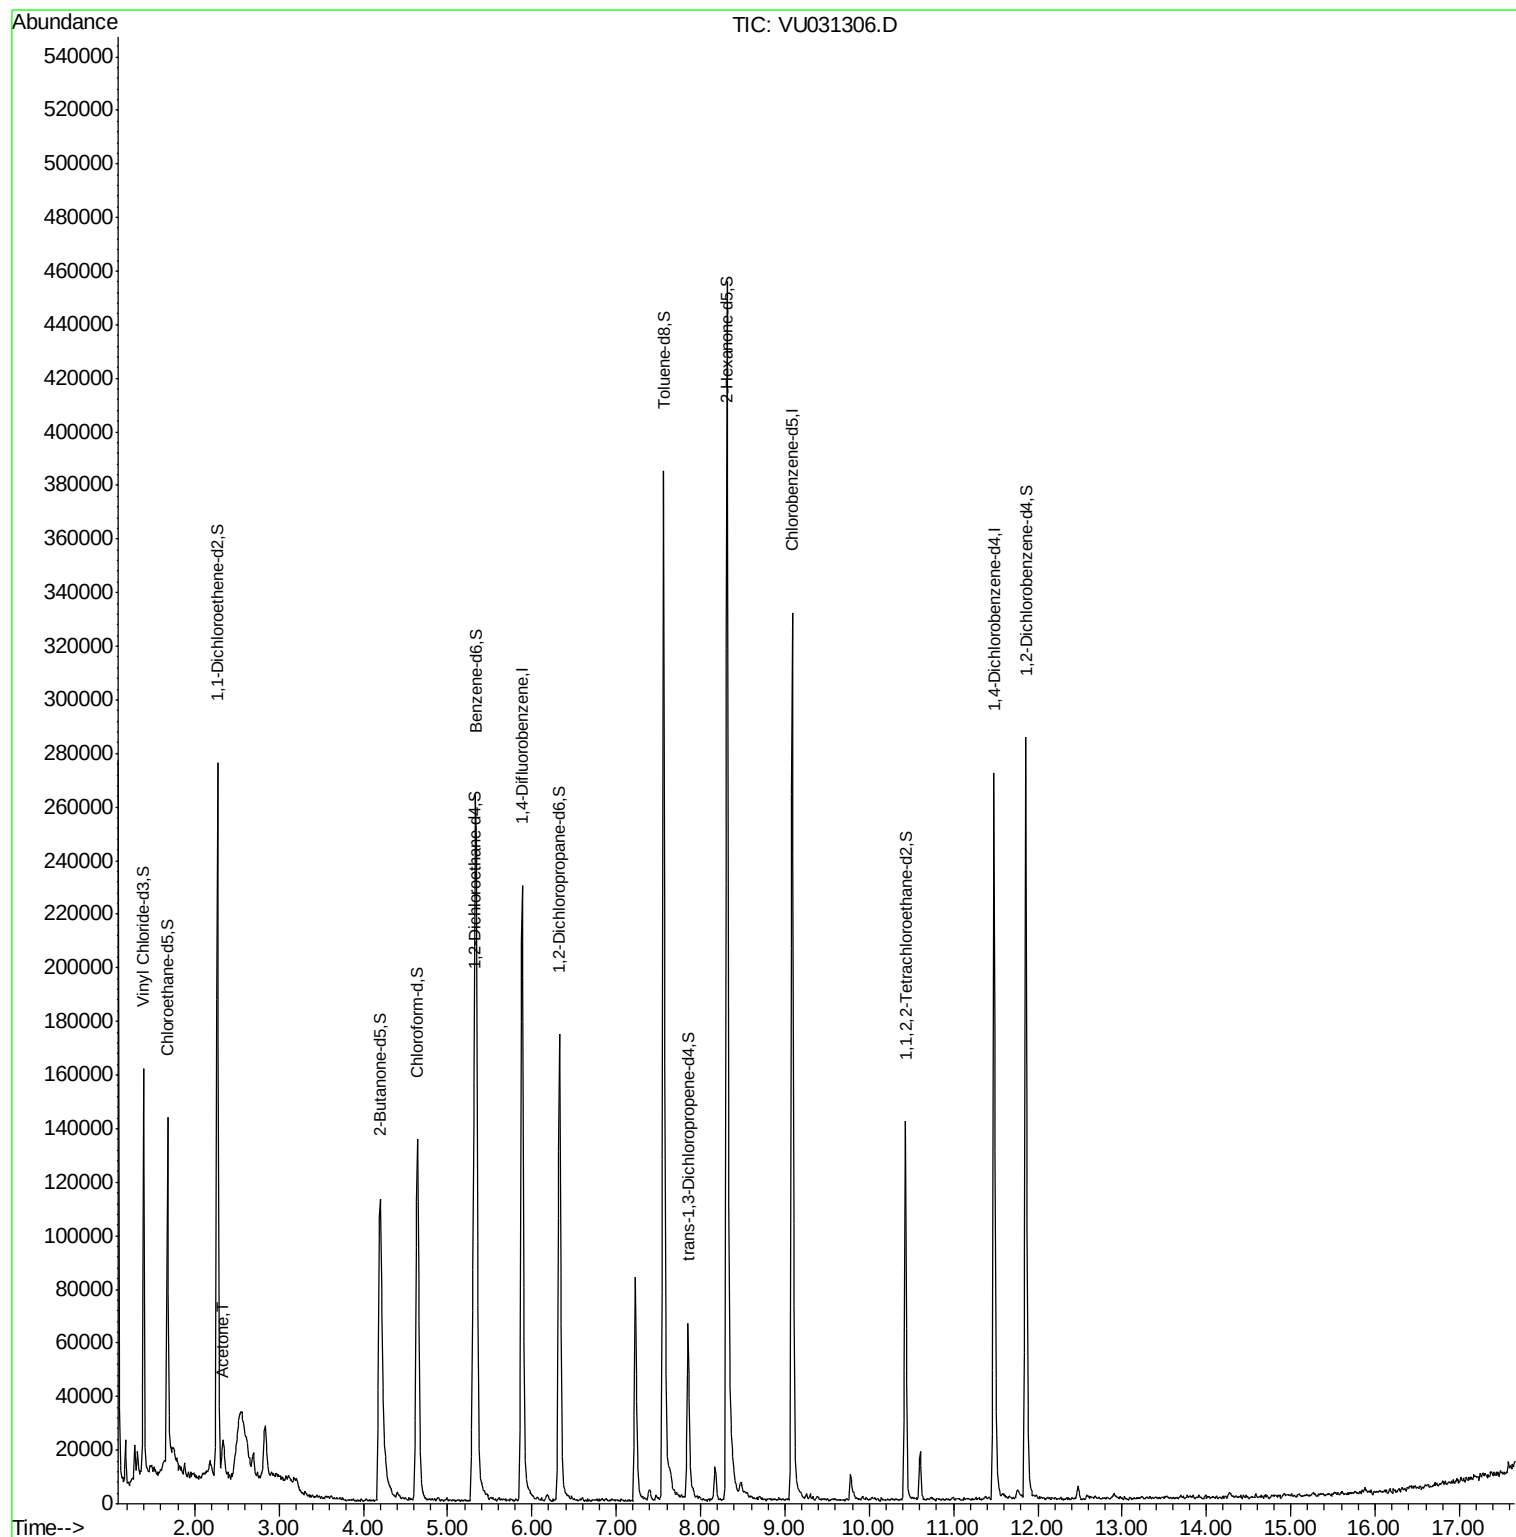

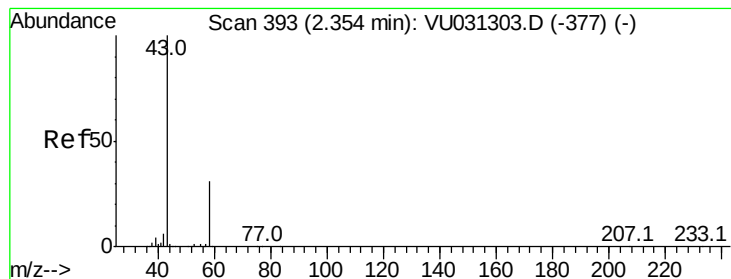

#13
 Acetone
 Concen: 3.076 ug/L
 RT: 2.34 min Scan# 389
 Delta R.T. -0.02 min
 Lab File: VU031306.D
 Acq: 18 Apr 2019 14:52

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XE3

Tot Ion: 43 Resp: 14711
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 64.4

