

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041919\
 Data File : VU031308.D
 Acq On : 18 Apr 2019 15:41
 Operator : JC/SP
 Sample : K2410-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD1

Quant Time: Apr 19 05:10:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 19 04:38:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	200077	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	196125	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	93042	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	105252	4.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.40%
7) Chloroethane-d5	1.68	69	82111	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.40%
11) 1,1-Dichloroethene-d2	2.27	63	155128	3.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.20%
20) 2-Butanone-d5	4.20	46	212562	49.29	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.58%
24) Chloroform-d	4.64	84	136305	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.31	65	76381	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
32) Benzene-d6	5.34	84	262054	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.33	67	89317	5.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.00%
41) Toluene-d8	7.56	98	222351	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.85	79	32204	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
46) 2-Hexanone-d5	8.31	63	154838	48.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.36%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	70546	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	100181	5.52	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.40%


Target Compounds					Ovalue
13) Acetone	2.33	43	36771	7.665 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041919\
Data File : VU031308.D
Acq On : 18 Apr 2019 15:41
Operator : JC/SP
Sample : K2410-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD1

Quant Time: Apr 19 05:10:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 19 04:38:37 2019
Response via : Initial Calibration

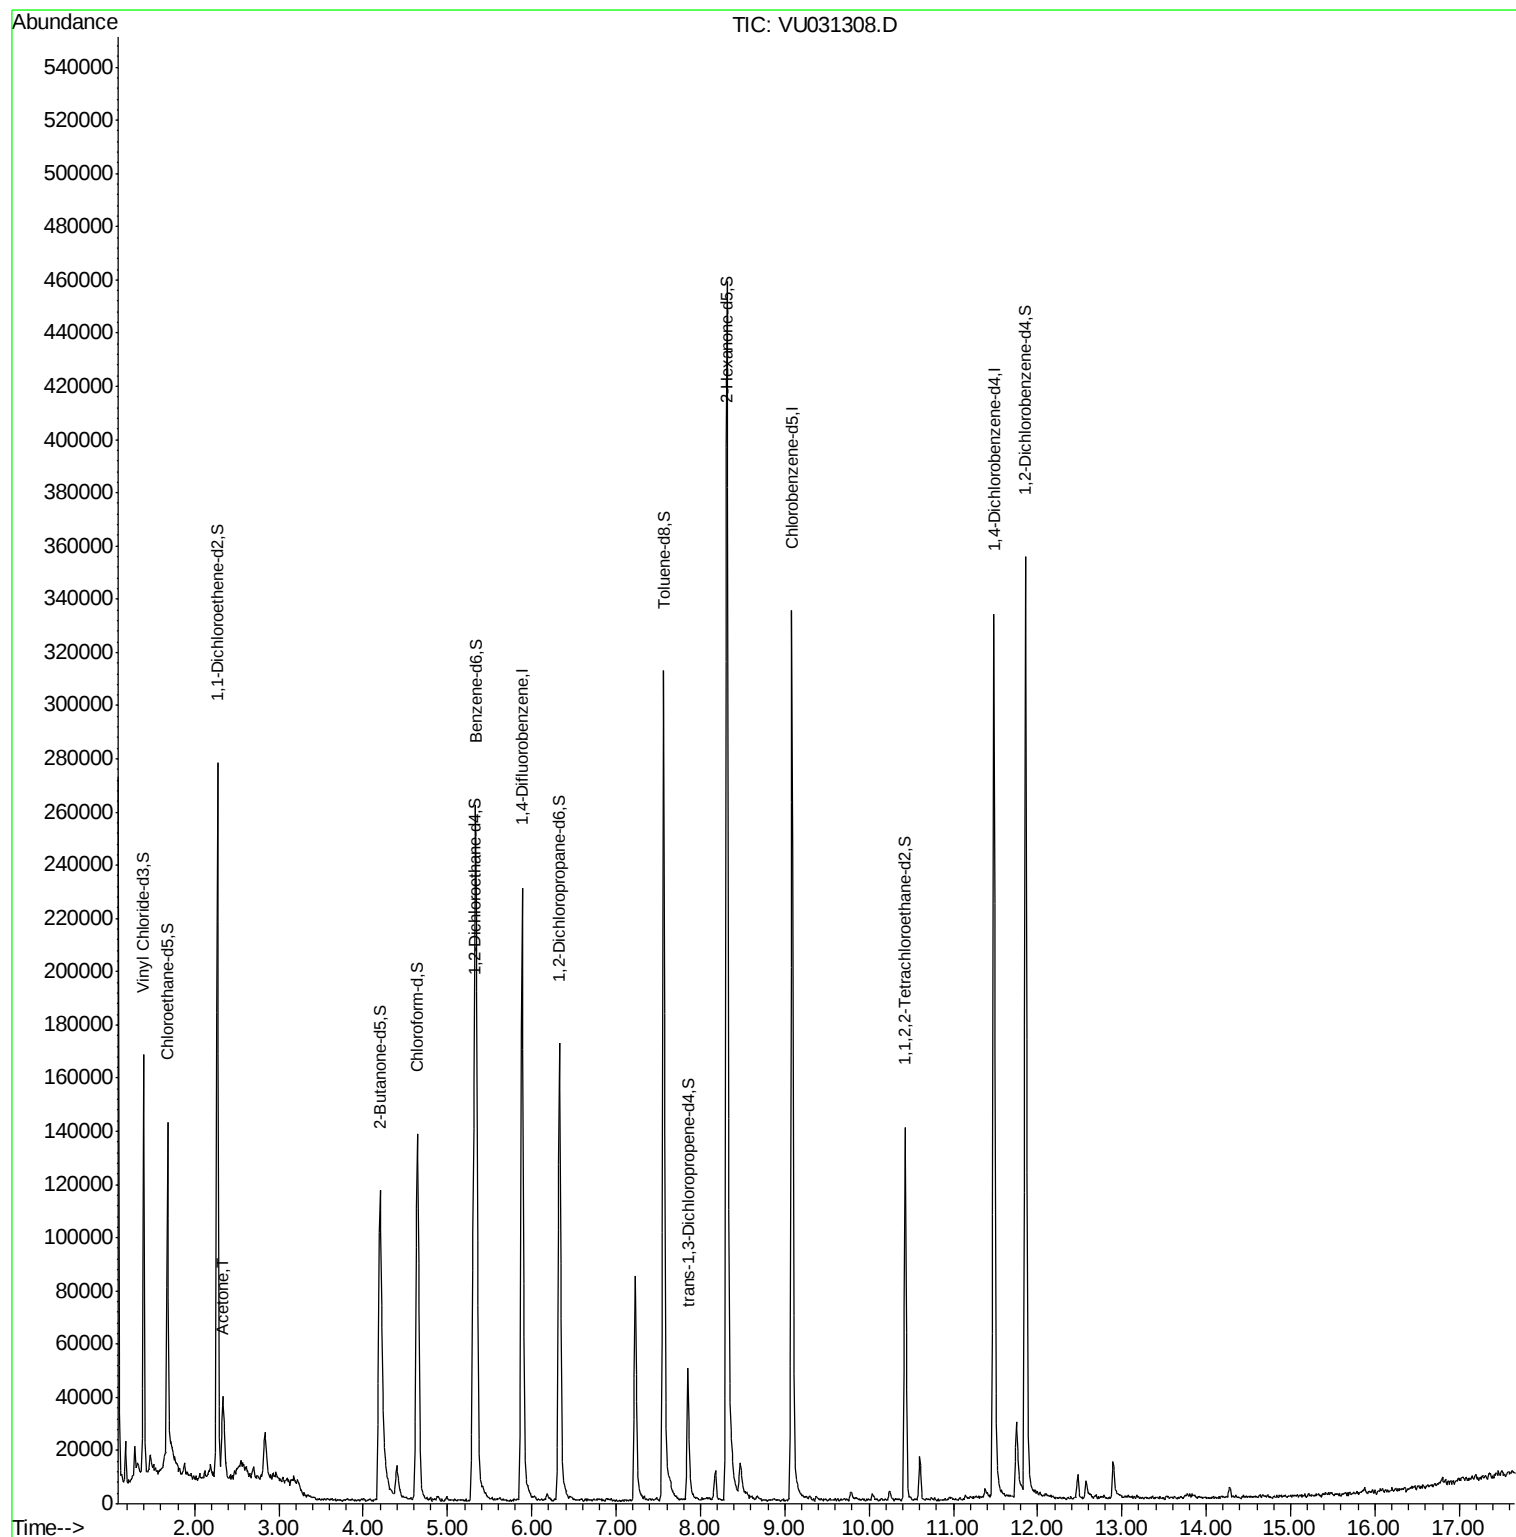

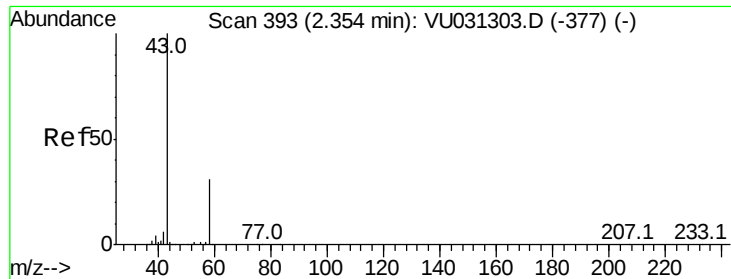

#13

Acetone

Concen: 7.665 ug/L

RT: 2.33 min Scan# 387

Delta R.T. -0.02 min

Lab File: VU031308.D

Acq: 18 Apr 2019 15:41

Instrument :

MSVOA_U

ClientSampleId :

C0XD1

Tot Ion: 43 Resp: 36771

Ion Ratio Lower Upper

43 100

58 31.7 0.0 64.4

