

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041919\
 Data File : VU031332.D
 Acq On : 19 Apr 2019 03:12
 Operator : JC/SP
 Sample : K2478-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD0

Quant Time: Apr 19 08:09:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Apr 19 07:47:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	246075	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	246811	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	92448	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	93950	3.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.80%
7) Chloroethane-d5	1.68	69	80960	3.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.40%
11) 1,1-Dichloroethene-d2	2.27	63	142759	2.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.40%#
20) 2-Butanone-d5	4.21	46	302854	57.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.20%
24) Chloroform-d	4.65	84	179638	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	5.31	65	98548	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.20%
32) Benzene-d6	5.34	84	342240	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.33	67	116193	5.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.60%
41) Toluene-d8	7.56	98	264699	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
43) trans-1,3-Dichloropropene-	7.85	79	38922	4.50	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.00%
46) 2-Hexanone-d5	8.31	63	197994	49.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.92%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	97762	5.39	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	99688	5.53	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.60%


Target Compounds					Ovalue
13) Acetone	2.34	43	47956	8.128 ug/L	98
34) Trichloroethene	6.18	95	4206	0.186 ug/L #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041919\
Data File : VU031332.D
Acq On : 19 Apr 2019 03:12
Operator : JC/SP
Sample : K2478-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD0

Quant Time: Apr 19 08:09:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Apr 19 07:47:43 2019
Response via : Initial Calibration

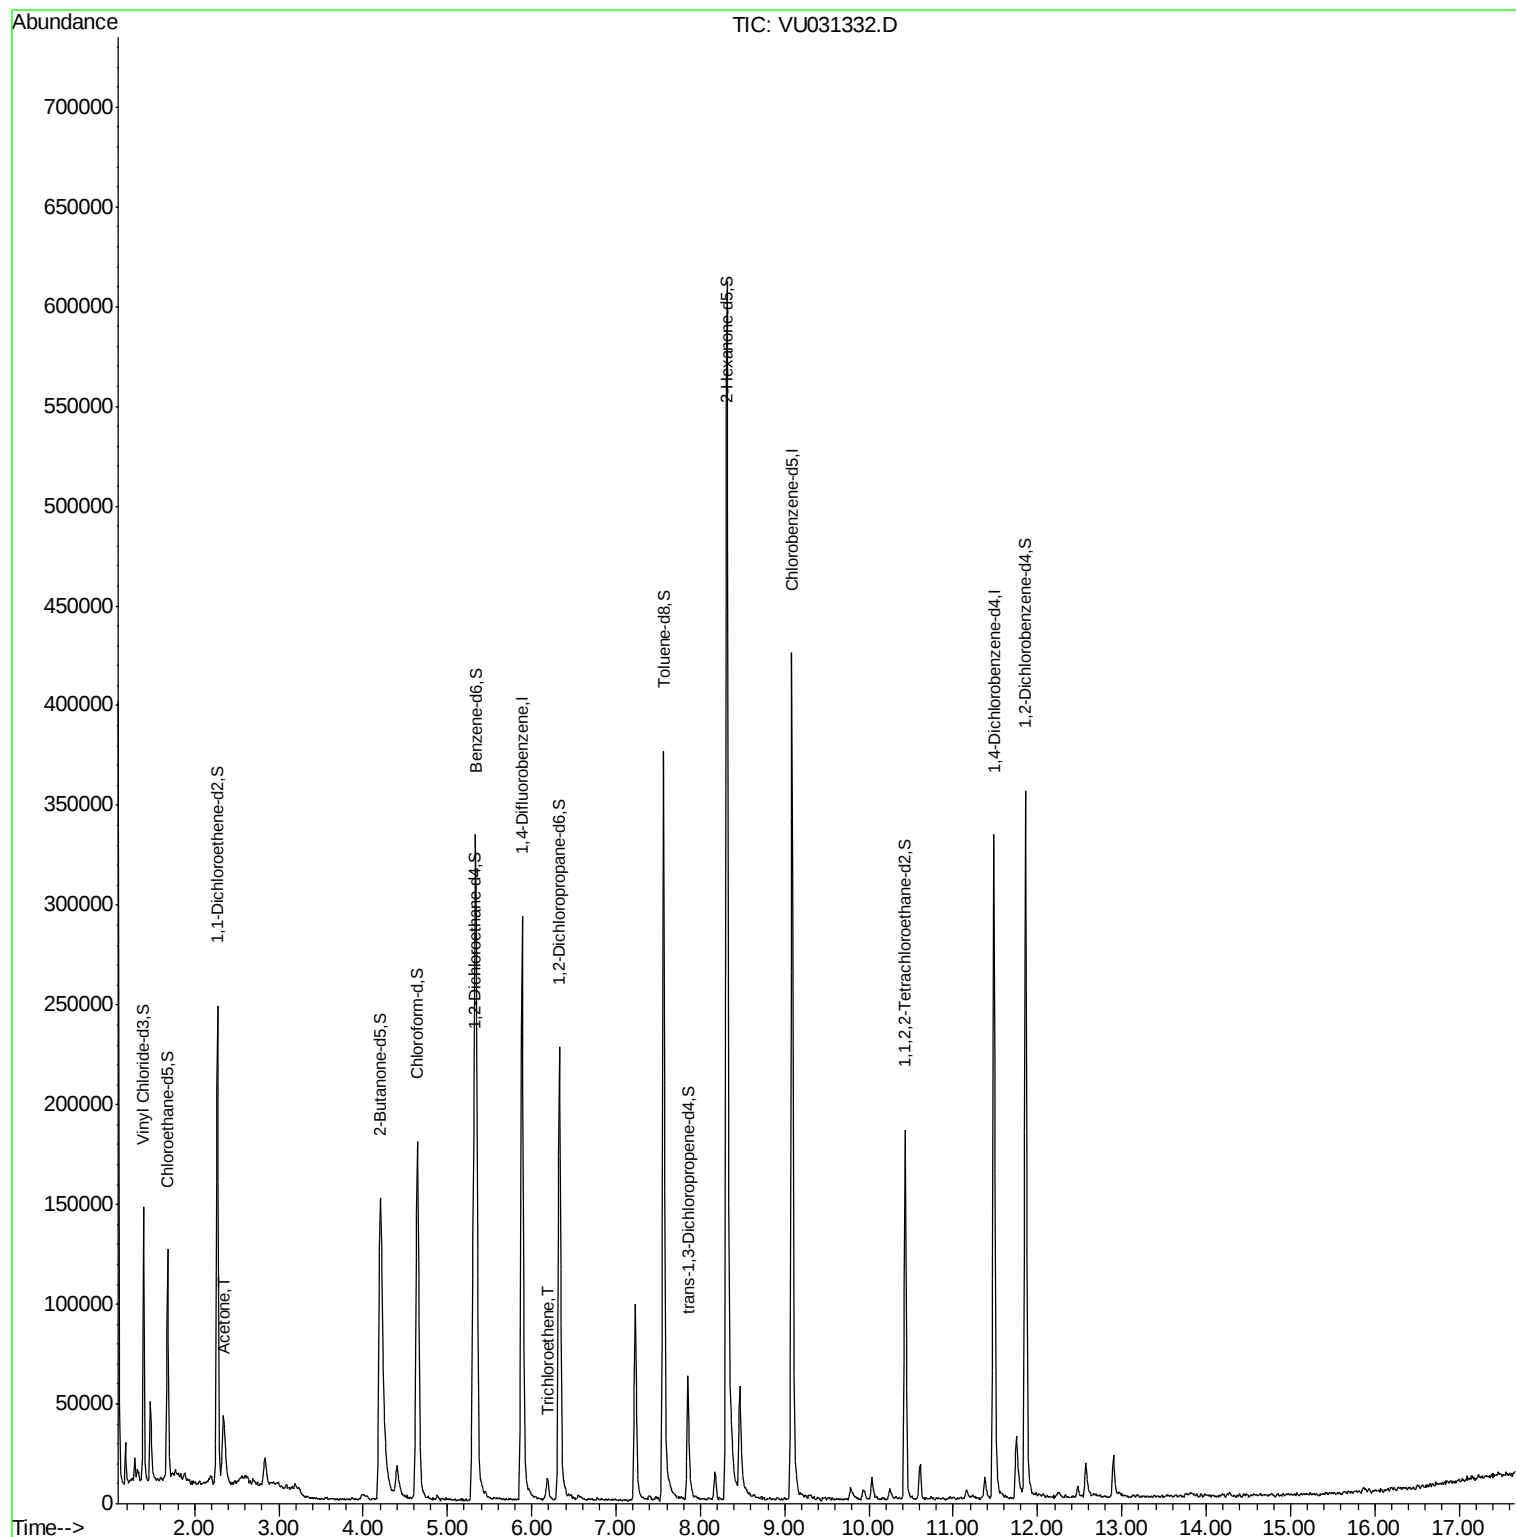

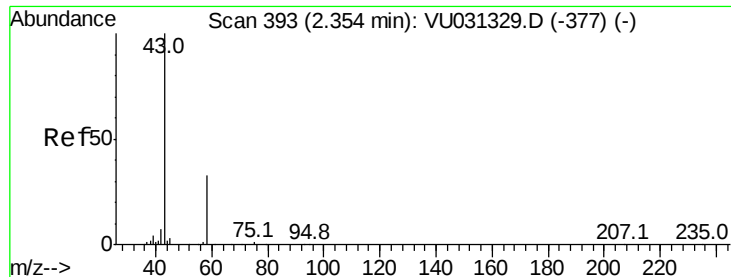

#13

Acetone

Concen: 8.128 ug/L

RT: 2.34 min Scan# 390

Delta R.T. -0.01 min

Lab File: VU031332.D

Acq: 19 Apr 2019 03:12

Instrument :

MSVOA_U

ClientSampleId :


C0XD0

Tot Ion: 43 Resp: 47956




Ion Ratio Lower Upper

43 100

58 33.1 0.0 64.4

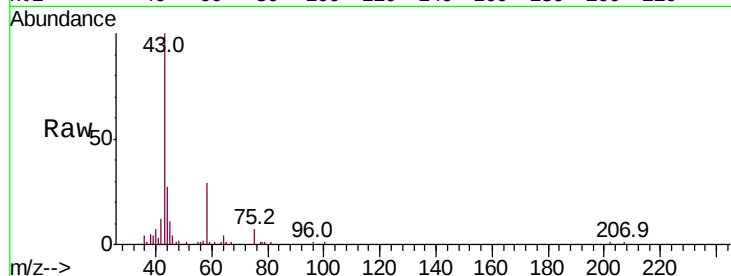

Abundance Ion 43.05 (42.75 to 43.75): VU031332.D (-377) (-)

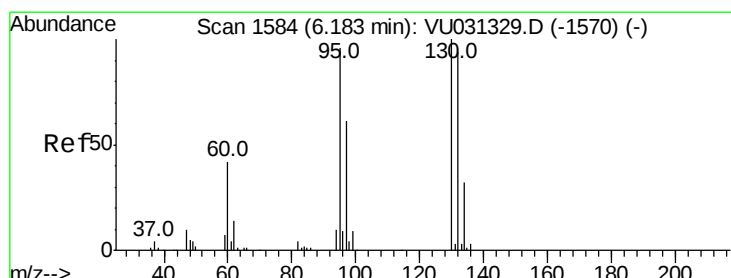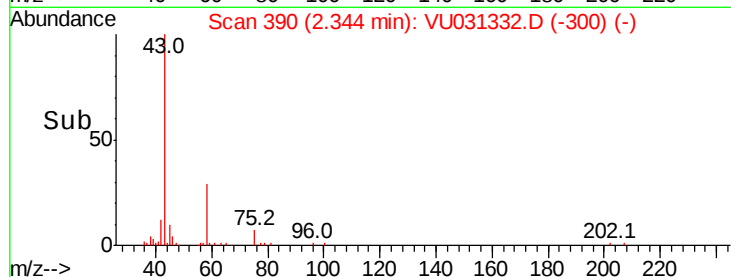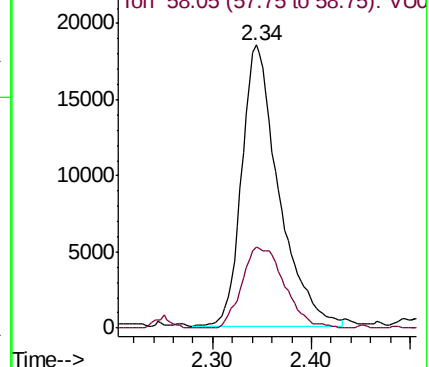

#34

Trichloroethene

Concen: 0.186 ug/L

RT: 6.18 min Scan# 1584

Delta R.T. 0.00 min

Lab File: VU031332.D

Acq: 19 Apr 2019 03:12

Tgt Ion: 95 Resp: 4206


Ion Ratio Lower Upper

95 100

97 37.7 46.8 86.8#

132 73.6 65.8 122.2

130 80.0 69.5 129.1

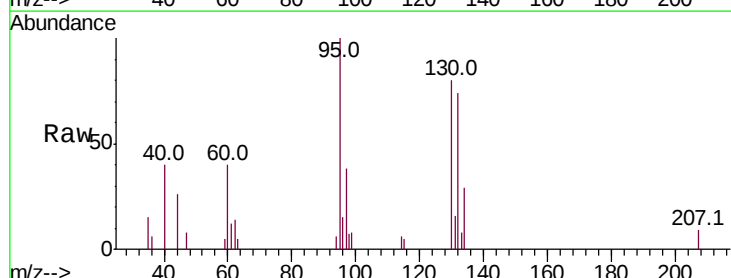

Abundance Ion 95.00 (94.70 to 95.70): VU031332.D (-1491) (-)

