


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041919\
Data File : VU031296.D
Acq On : 18 Apr 2019 09:19
Operator : JC/SP
Sample : BFB41
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Apr 20 05:39:07 2019

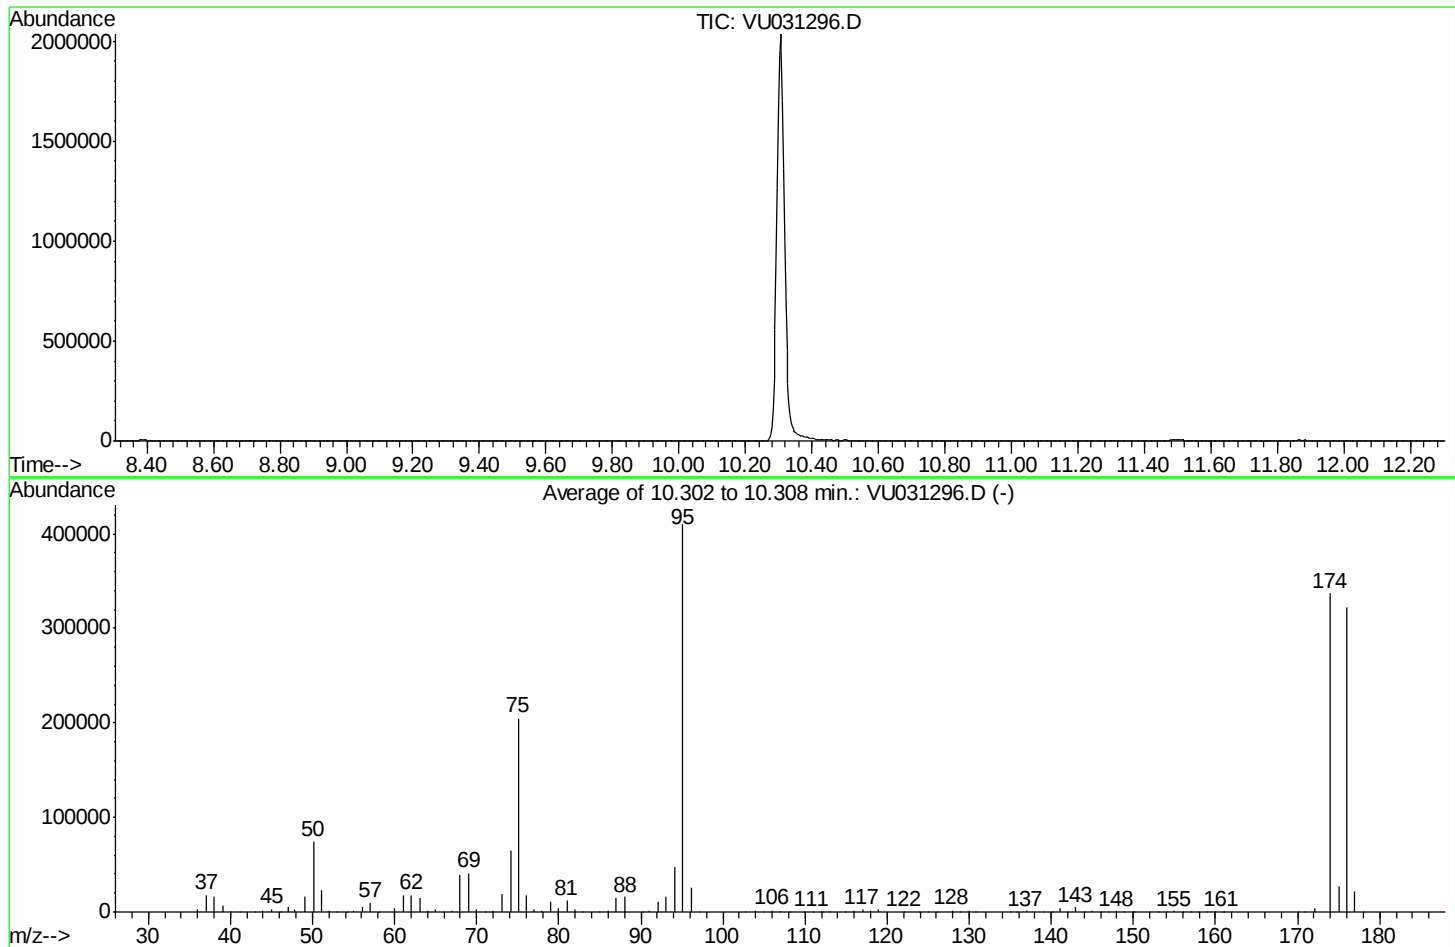

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	74440	PASS
75	95	30	80	49.9	204501	PASS
95	95	100	100	100.0	410005	PASS
96	95	5	9	6.3	25696	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.2	337045	PASS
175	174	5	9	7.9	26757	PASS
176	174	95	101	95.7	322666	PASS
177	176	5	9	6.6	21429	PASS

Scan 2851 (10.257 min): VU031296.D
BFB41

m/z	Abundance
40.00	807.0
43.30	107.0
44.00	685.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	3494.0
37.10	17232.0
38.00	16339.0
39.10	7422.0
40.00	989.0
43.00	226.0
44.00	2044.0
45.10	3124.0
46.00	596.0
47.00	5228.0
47.90	2283.0
49.10	15597.0
50.10	74528.0
51.10	22336.0
52.00	1092.0
53.00	452.0
54.20	152.0
55.00	944.0
56.00	5623.0
57.10	9629.0
58.10	492.0
60.10	3646.0
61.10	17976.0
62.00	17792.0
63.10	15007.0
64.10	2238.0
65.00	2763.0
65.90	328.0
67.00	1104.0
68.00	39344.0
69.10	39864.0
70.00	2728.0
71.00	124.0
72.00	1988.0
73.10	18880.0
74.10	64080.0
75.10	202048.0
76.10	17792.0
77.00	2378.0
77.90	1472.0
79.00	12017.0
80.00	3791.0
81.00	11707.0
82.00	2541.0
82.90	340.0
84.90	102.0
86.00	954.0
87.00	15148.0
88.10	15997.0
91.00	1337.0
92.00	10613.0
93.10	16448.0
94.10	46808.0
95.10	400128.0
96.10	24944.0
97.10	589.0
102.80	327.0
104.00	1278.0
104.90	535.0
106.00	1659.0
107.00	249.0
108.10	122.0
109.90	245.0
110.90	263.0
111.80	174.0
112.20	185.0
113.00	244.0
114.90	455.0
116.00	1594.0
117.00	2679.0
118.00	1759.0
119.00	2220.0
122.00	153.0
123.90	231.0
125.00	101.0
126.10	113.0
127.90	1462.0
129.00	539.0
130.00	1501.0
130.80	437.0
135.00	673.0
137.00	899.0
140.10	325.0
141.10	3328.0
142.10	472.0
143.00	5386.0
144.10	558.0
145.00	1932.0
146.00	435.0
147.10	186.0
148.00	808.0
148.90	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

149.90	560.0
152.00	307.0
153.00	288.0
154.00	168.0
155.00	895.0
156.00	131.0
157.10	753.0
157.90	107.0
158.90	430.0
160.80	441.0
172.10	4031.0
174.00	323008.0
175.10	26080.0
176.00	307968.0
177.00	20424.0
178.00	556.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	3412.0
37.10	18424.0
38.00	16768.0
39.10	7452.0
40.00	911.0
43.00	288.0
44.00	2186.0
45.00	3187.0
46.10	694.0
47.00	5115.0
47.90	2339.0
49.10	16400.0
50.10	77184.0
51.10	23656.0
52.10	1129.0
53.00	456.0
55.10	1112.0
56.00	5434.0
57.10	9757.0
58.00	483.0
60.00	3594.0
61.10	18328.0
62.10	18696.0
63.10	15806.0
64.10	2121.0
65.10	2823.0
65.90	331.0
67.00	1192.0
68.00	41088.0
69.10	42456.0
70.00	3111.0
72.00	2028.0
73.10	19536.0
74.10	66648.0
75.10	211008.0
76.10	18240.0
77.00	2527.0
77.90	1591.0
79.00	11803.0
80.00	3805.0
81.00	12367.0
82.00	2570.0
82.90	390.0
86.00	1046.0
87.00	15812.0
88.10	16480.0
90.20	104.0
91.00	1238.0
92.10	11170.0
93.10	17456.0
94.10	48776.0
95.10	423936.0
96.10	26384.0
97.10	555.0
102.80	328.0
104.00	1582.0
104.90	557.0
106.00	1664.0
107.00	262.0
109.80	243.0
110.90	313.0
111.80	214.0
113.00	288.0
114.90	524.0
115.90	1637.0
117.00	2777.0
118.00	1870.0
119.00	2336.0
122.10	227.0
123.90	243.0
125.00	171.0
127.90	1555.0
128.90	647.0
130.00	1445.0
130.90	431.0
135.00	698.0
135.70	109.0
137.00	997.0
140.10	373.0
141.10	3721.0
142.00	470.0
143.00	5237.0
144.10	455.0
145.00	1881.0
146.00	613.0
147.00	229.0
148.00	849.0
148.90	213.0
150.10	596.0
152.00	222.0
153.00	304.0
153.90	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

155.00	884.0
156.10	118.0
157.00	705.0
157.90	114.0
159.00	446.0
159.90	154.0
160.80	452.0
172.10	4121.0
174.00	348096.0
175.10	27616.0
176.00	333120.0
177.00	22280.0
178.00	630.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	2989.0
37.10	17256.0
38.00	15252.0
39.10	6718.0
40.10	885.0
41.10	129.0
43.00	281.0
44.00	2275.0
45.00	2986.0
46.10	638.0
47.00	4613.0
47.90	1882.0
49.00	15466.0
50.10	71608.0
51.10	22384.0
52.00	989.0
53.00	350.0
55.10	1150.0
56.10	4804.0
57.10	9420.0
58.00	441.0
60.00	3186.0
61.10	17288.0
62.10	18008.0
63.10	14983.0
64.10	1755.0
65.10	2616.0
66.00	319.0
67.10	1058.0
68.00	38200.0
69.10	40064.0
70.00	3075.0
72.00	1911.0
73.00	17648.0
74.10	64032.0
75.10	200448.0
76.10	16768.0
77.00	2275.0
78.00	1649.0
79.00	10273.0
80.00	3390.0
81.00	11811.0
82.00	2285.0
82.90	352.0
85.90	936.0
87.00	15084.0
88.10	15178.0
91.00	1130.0
92.10	10689.0
93.10	16688.0
94.10	45744.0
95.10	405952.0
96.10	25760.0
97.10	474.0
102.70	224.0
104.00	1716.0
104.90	549.0
106.00	1505.0
106.90	320.0
109.80	200.0
110.90	272.0
111.90	200.0
113.00	292.0
114.90	493.0
115.90	1513.0
117.00	2660.0
117.90	1638.0
119.00	2245.0
122.10	255.0
124.00	259.0
124.90	194.0
127.90	1417.0
128.90	724.0
130.00	1237.0
130.90	465.0
135.00	645.0
136.90	935.0
139.00	100.0
139.90	352.0
141.00	3947.0
141.90	441.0
143.00	4651.0
144.20	279.0
145.00	1603.0
146.00	659.0
147.00	258.0
147.90	973.0
148.90	200.0
150.00	582.0
152.00	108.0
153.00	269.0
153.90	313.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

154.90	823.0
156.90	677.0
158.00	158.0
159.00	487.0
159.90	140.0
161.00	378.0
170.10	115.0
170.90	571.0
172.10	3875.0
174.00	340032.0
175.10	26576.0
176.00	326912.0
177.00	21584.0
178.00	573.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41