

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048132.D
 Acq On : 19 Apr 2022 13:56
 Operator : SY/MD
 Sample : N2419-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	101	rVB	161049	191848	15.59%	1.902%
2	1.916	171	179	201	rVB	123488	175357	14.25%	1.738%
3	2.571	370	383	396	rBV	273990	452179	36.74%	4.483%
4	2.723	427	430	433	rBV2	340	223	0.02%	0.002%
5	2.797	444	453	463	rBV4	1065	1927	0.16%	0.019%
6	2.944	497	499	504	rBV2	375	329	0.03%	0.003%
7	3.047	525	531	533	rBV3	741	680	0.06%	0.007%
8	3.108	544	550	552	rBV	265	280	0.02%	0.003%
9	3.189	566	575	586	rBV5	1179	2648	0.22%	0.026%
10	3.475	660	664	668	rBV	399	342	0.03%	0.003%
11	3.510	671	675	677	rBV	214	200	0.02%	0.002%
12	3.549	684	687	690	rBV2	328	258	0.02%	0.003%
13	3.610	701	706	709	rBV2	294	275	0.02%	0.003%
14	3.633	709	713	715	rVV2	207	195	0.02%	0.002%
15	3.649	715	718	725	rVB2	209	256	0.02%	0.003%
16	3.694	725	732	735	rVB2	230	281	0.02%	0.003%
17	4.324	925	928	933	rBV2	193	222	0.02%	0.002%
18	4.388	944	948	952	rBV2	234	211	0.02%	0.002%
19	4.497	976	982	983	rBV2	216	225	0.02%	0.002%
20	4.626	1005	1022	1069	rBV	122805	322898	26.23%	3.201%
21	4.806	1074	1078	1079	rBV	609	420	0.03%	0.004%
22	5.067	1142	1159	1181	rVV	227581	496666	40.35%	4.924%
23	5.298	1223	1231	1236	rVB3	623	912	0.07%	0.009%
24	5.369	1249	1253	1255	rBV2	302	195	0.02%	0.002%
25	5.587	1317	1321	1324	rBV	344	283	0.02%	0.003%
26	5.613	1324	1329	1331	rVV2	192	204	0.02%	0.002%
27	5.729	1342	1365	1397	rBV2	453962	1230830	100.00%	12.202%
28	6.112	1482	1484	1489	rVB4	357	277	0.02%	0.003%
29	6.173	1499	1503	1505	rBV3	256	194	0.02%	0.002%
30	6.253	1512	1528	1553	rBV	409825	785792	63.84%	7.790%
31	6.494	1598	1603	1607	rBV4	298	366	0.03%	0.004%
32	6.533	1608	1615	1617	rBV5	1391	1592	0.13%	0.016%
33	6.591	1631	1633	1639	rBV3	413	339	0.03%	0.003%
34	6.693	1650	1665	1687	rBV	284110	553011	44.93%	5.482%
35	6.880	1721	1723	1726	rBV2	464	342	0.03%	0.003%
36	6.922	1731	1736	1739	rVV2	347	258	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048132.D
 Acq On : 19 Apr 2022 13:56
 Operator : SY/MD
 Sample : N2419-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.189	1811	1819	1833	rVB5	2613	4885	0.40%	0.048%
38	7.568	1925	1937	1955	rBV	144590	257038	20.88%	2.548%
39	7.687	1968	1974	1976	rBV3	1407	1485	0.12%	0.015%
40	7.800	2002	2009	2015	rBV3	1006	1589	0.13%	0.016%
41	7.902	2027	2041	2056	rBV	549525	956706	77.73%	9.484%
42	8.128	2108	2111	2114	rBV	501	363	0.03%	0.004%
43	8.182	2114	2128	2147	rBV	96380	168665	13.70%	1.672%
44	8.346	2175	2179	2183	rVB3	350	343	0.03%	0.003%
45	8.475	2212	2219	2228	rVV3	2865	4357	0.35%	0.043%
46	8.555	2240	2244	2248	rBV2	212	210	0.02%	0.002%
47	8.581	2248	2252	2257	rVB3	258	221	0.02%	0.002%
48	8.639	2257	2270	2302	rBV	345391	648673	52.70%	6.431%
49	8.787	2312	2316	2318	rBV3	1080	1008	0.08%	0.010%
50	8.841	2330	2333	2336	rBV2	490	336	0.03%	0.003%
51	8.925	2356	2359	2364	rVV2	323	298	0.02%	0.003%
52	8.960	2366	2370	2375	rVV3	271	231	0.02%	0.002%
53	8.999	2378	2382	2385	rVB2	381	267	0.02%	0.003%
54	9.028	2385	2391	2394	rBV2	363	432	0.04%	0.004%
55	9.166	2427	2434	2439	rVB3	704	901	0.07%	0.009%
56	9.208	2439	2447	2450	rBV	310	407	0.03%	0.004%
57	9.227	2450	2453	2456	rVV	327	215	0.02%	0.002%
58	9.301	2473	2476	2479	rBV2	325	203	0.02%	0.002%
59	9.420	2500	2513	2548	rBV	633734	1083361	88.02%	10.740%
60	9.642	2577	2582	2583	rVV	426	335	0.03%	0.003%
61	9.668	2587	2590	2593	rVV2	273	202	0.02%	0.002%
62	9.700	2593	2600	2606	rVB4	1075	1437	0.12%	0.014%
63	9.812	2630	2635	2639	rBV2	208	249	0.02%	0.002%
64	10.031	2701	2703	2709	rVV2	222	243	0.02%	0.002%
65	10.488	2840	2845	2846	rBV3	441	458	0.04%	0.005%
66	10.568	2867	2870	2878	rBV4	294	261	0.02%	0.003%
67	10.639	2889	2892	2896	rVV3	774	761	0.06%	0.008%
68	10.674	2896	2903	2913	rVB4	2683	4016	0.33%	0.040%
69	10.758	2917	2929	2950	rBV	421580	696457	56.58%	6.904%
70	10.899	2959	2973	2985	rVB4	5717	10300	0.84%	0.102%
71	10.957	2985	2991	2994	rBV2	436	415	0.03%	0.004%
72	11.092	3027	3033	3037	rBV3	559	688	0.06%	0.007%
73	11.205	3066	3068	3072	rBV	437	328	0.03%	0.003%
74	11.275	3086	3090	3095	rBV2	365	453	0.04%	0.004%
75	11.468	3139	3150	3161	rVB8	2115	4708	0.38%	0.047%
76	11.552	3173	3176	3179	rVV2	262	199	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048132.D
 Acq On : 19 Apr 2022 13:56
 Operator : SY/MD
 Sample : N2419-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0JA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.578	3180	3184	3186	rVV2	464	335	0.03%	0.003%
78	11.594	3187	3189	3192	rVB2	405	222	0.02%	0.002%
79	11.697	3214	3221	3227	rVB6	1479	2017	0.16%	0.020%
80	11.748	3230	3237	3245	rVB4	1242	1671	0.14%	0.017%
81	11.815	3245	3258	3284	rBV	661649	1054233	85.65%	10.451%
82	11.973	3303	3307	3316	rVB6	2179	2960	0.24%	0.029%
83	12.018	3317	3321	3323	rBV	419	260	0.02%	0.003%
84	12.066	3327	3336	3346	rBV3	11085	19016	1.54%	0.189%
85	12.150	3359	3362	3363	rBV3	380	244	0.02%	0.002%
86	12.195	3363	3376	3394	rVV	550267	902274	73.31%	8.945%
87	12.272	3397	3400	3404	rBV3	543	458	0.04%	0.005%
88	12.362	3425	3428	3429	rBV	495	258	0.02%	0.003%
89	12.394	3436	3438	3443	rVB3	350	275	0.02%	0.003%
90	12.690	3526	3530	3534	rBV2	322	317	0.03%	0.003%
91	12.896	3587	3594	3602	rVB5	4322	6061	0.49%	0.060%
92	12.944	3607	3609	3614	rVB2	514	346	0.03%	0.003%
93	12.970	3614	3617	3620	rBV	252	248	0.02%	0.002%
94	13.230	3690	3698	3708	rBV5	1491	2376	0.19%	0.024%
95	13.301	3713	3720	3722	rBV3	377	445	0.04%	0.004%
96	13.458	3765	3769	3772	rBV2	638	552	0.04%	0.005%
97	13.651	3827	3829	3831	rBV2	344	211	0.02%	0.002%
98	13.844	3881	3889	3899	rBV4	3450	5327	0.43%	0.053%
99	14.095	3959	3967	3978	rBV2	4058	6562	0.53%	0.065%
100	14.333	4035	4041	4054	rVB3	2658	4392	0.36%	0.044%




Sum of corrected areas: 10087279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048132.D
Acq On : 19 Apr 2022 13:56
Operator : SY/MD
Sample : N2419-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

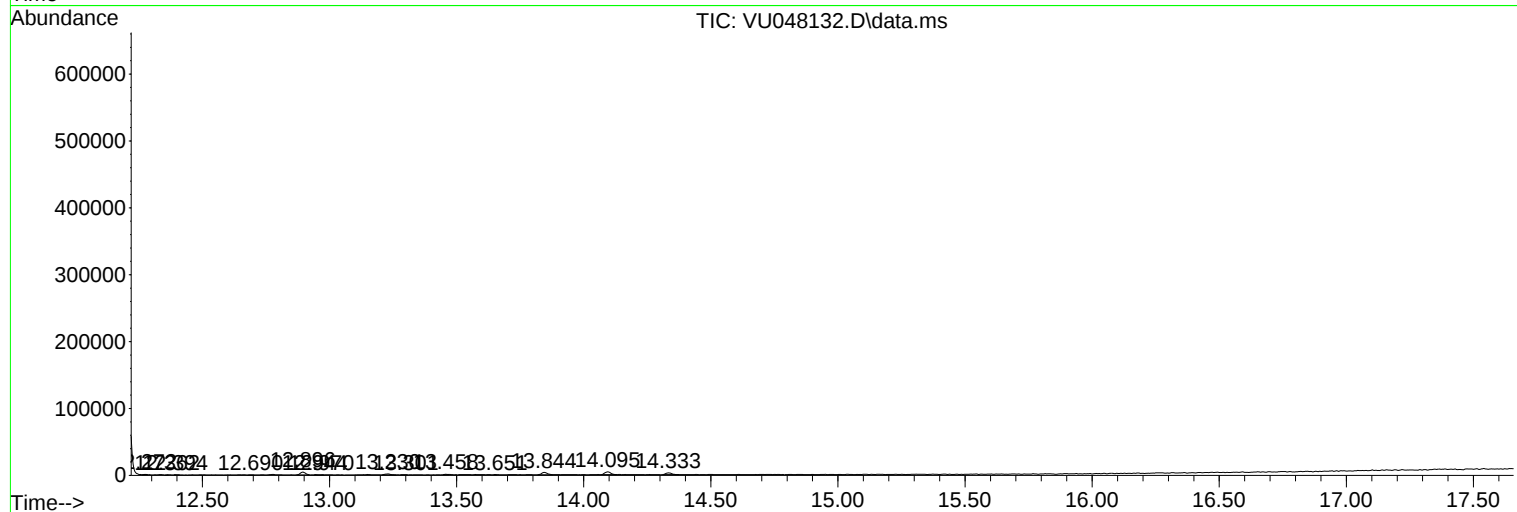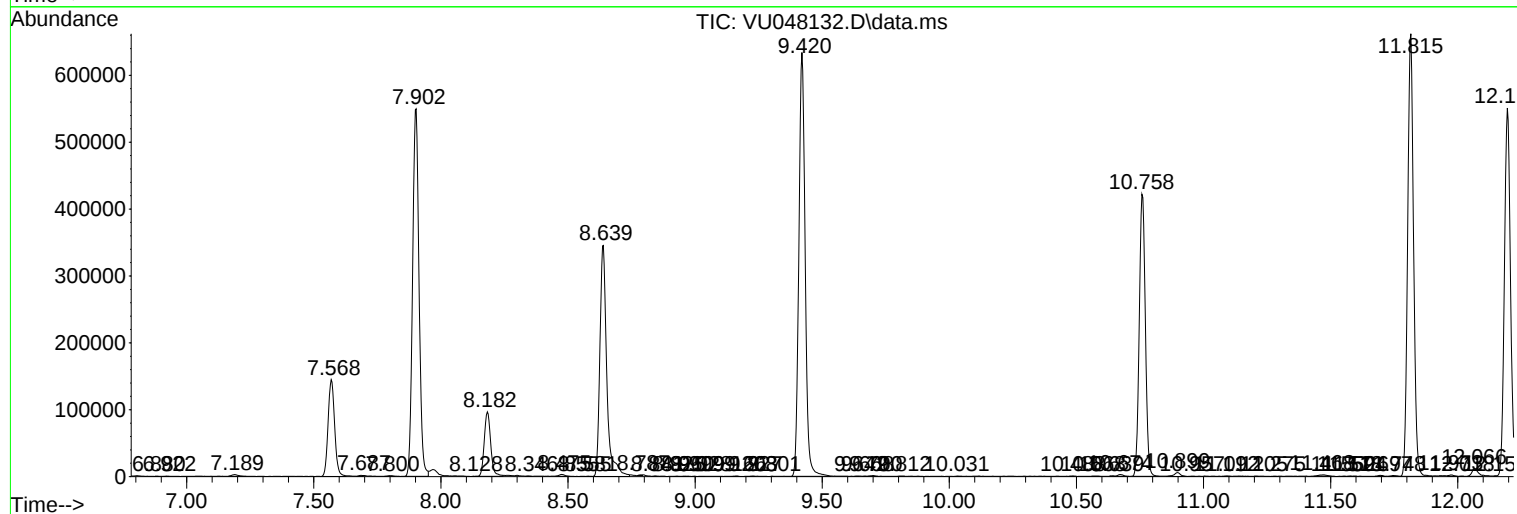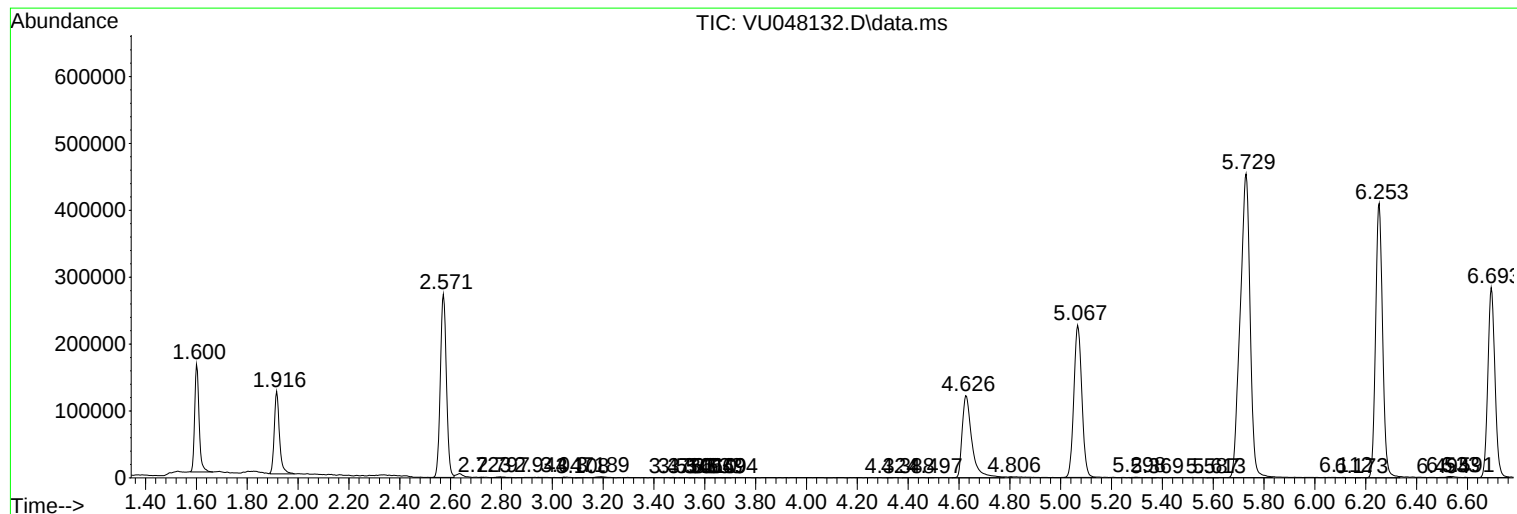

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048132.D
Acq On : 19 Apr 2022 13:56
Operator : SY/MD
Sample : N2419-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048132.D
Acq On : 19 Apr 2022 13:56
Operator : SY/MD
Sample : N2419-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0JA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc