

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048133.D
 Acq On : 19 Apr 2022 15:12
 Operator : SY/MD
 Sample : N2419-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048133.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rBV	159175	186673	15.62%	1.892%
2	1.915	171	179	203	rVB	120053	172065	14.40%	1.744%
3	2.571	370	383	403	rBV	263891	434248	36.34%	4.401%
4	2.796	444	453	460	rVB3	498	841	0.07%	0.009%
5	2.883	477	480	482	rBV2	237	173	0.01%	0.002%
6	2.951	498	501	503	rBV2	241	181	0.02%	0.002%
7	3.057	523	534	543	rVB4	2722	5192	0.43%	0.053%
8	3.192	565	576	582	rBV3	915	1658	0.14%	0.017%
9	3.343	620	623	628	rVB	288	221	0.02%	0.002%
10	3.417	639	646	650	rBV2	305	386	0.03%	0.004%
11	3.694	729	732	739	rBV2	191	249	0.02%	0.003%
12	3.761	749	753	757	rVB2	242	224	0.02%	0.002%
13	3.787	757	761	765	rBV2	231	206	0.02%	0.002%
14	3.996	823	826	830	rVB2	294	213	0.02%	0.002%
15	4.128	863	867	873	rVB	201	212	0.02%	0.002%
16	4.321	920	927	930	rBV2	148	212	0.02%	0.002%
17	4.626	1009	1022	1049	rBV	125004	312693	26.16%	3.169%
18	5.066	1143	1159	1180	rBV	217704	481606	40.30%	4.881%
19	5.224	1206	1208	1216	rVB3	313	311	0.03%	0.003%
20	5.292	1223	1229	1231	rBV5	546	573	0.05%	0.006%
21	5.359	1246	1250	1253	rBV2	234	190	0.02%	0.002%
22	5.394	1256	1261	1265	rBV2	183	236	0.02%	0.002%
23	5.594	1320	1323	1330	rVB	201	216	0.02%	0.002%
24	5.629	1330	1334	1339	rBV2	154	172	0.01%	0.002%
25	5.729	1343	1365	1395	rBV2	440199	1195119	100.00%	12.111%
26	5.973	1439	1441	1444	rBV2	336	201	0.02%	0.002%
27	6.089	1473	1477	1480	rVB3	257	254	0.02%	0.003%
28	6.115	1480	1485	1486	rBV2	494	330	0.03%	0.003%
29	6.182	1504	1506	1512	rVB2	391	295	0.02%	0.003%
30	6.253	1512	1528	1556	rBV	407550	779624	65.23%	7.901%
31	6.414	1577	1578	1585	rVB	426	222	0.02%	0.002%
32	6.533	1607	1615	1624	rBV3	1842	2888	0.24%	0.029%
33	6.597	1632	1635	1639	rVV2	378	271	0.02%	0.003%
34	6.616	1639	1641	1646	rVB2	270	175	0.01%	0.002%
35	6.693	1650	1665	1688	rBV	275793	538770	45.08%	5.460%
36	6.806	1698	1700	1703	rVB3	408	208	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048133.D
 Acq On : 19 Apr 2022 15:12
 Operator : SY/MD
 Sample : N2419-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.854	1713	1715	1718	rVV	370	182	0.02%	0.002%
38	7.037	1769	1772	1774	rBV2	347	253	0.02%	0.003%
39	7.192	1809	1820	1830	rVB4	2267	4296	0.36%	0.044%
40	7.234	1830	1833	1841	rVB2	193	213	0.02%	0.002%
41	7.568	1924	1937	1968	rBV	131773	235563	19.71%	2.387%
42	7.693	1973	1976	1983	rVB2	1367	1428	0.12%	0.014%
43	7.790	2003	2006	2008	rBV2	406	275	0.02%	0.003%
44	7.902	2027	2041	2057	rBV	498904	868585	72.68%	8.802%
45	8.182	2113	2128	2149	rBV	94106	162573	13.60%	1.647%
46	8.333	2173	2175	2178	rVB2	345	181	0.02%	0.002%
47	8.478	2214	2220	2224	rVV2	666	647	0.05%	0.007%
48	8.594	2251	2256	2257	rBV2	314	197	0.02%	0.002%
49	8.635	2257	2269	2316	rVV	377494	713062	59.66%	7.226%
50	8.864	2336	2340	2344	rVB2	468	411	0.03%	0.004%
51	8.883	2344	2346	2348	rBV	501	273	0.02%	0.003%
52	8.925	2355	2359	2362	rVB2	237	179	0.01%	0.002%
53	8.999	2378	2382	2386	rVB2	324	296	0.02%	0.003%
54	9.166	2429	2434	2438	rVV2	376	401	0.03%	0.004%
55	9.259	2459	2463	2466	rBV3	376	287	0.02%	0.003%
56	9.343	2484	2489	2494	rBV2	332	354	0.03%	0.004%
57	9.420	2499	2513	2554	rBV	620773	1059840	88.68%	10.740%
58	9.642	2579	2582	2589	rBV3	363	406	0.03%	0.004%
59	9.687	2592	2596	2597	rVV2	502	336	0.03%	0.003%
60	9.697	2597	2599	2609	rVB3	788	780	0.07%	0.008%
61	9.774	2619	2623	2626	rBV	260	180	0.02%	0.002%
62	9.861	2645	2650	2654	rVB2	273	255	0.02%	0.003%
63	9.960	2678	2681	2687	rVB2	237	246	0.02%	0.002%
64	10.008	2687	2696	2698	rBV	393	369	0.03%	0.004%
65	10.053	2706	2710	2714	rBV	230	202	0.02%	0.002%
66	10.233	2762	2766	2768	rVB	339	245	0.02%	0.002%
67	10.250	2768	2771	2774	rBV2	333	255	0.02%	0.003%
68	10.433	2823	2828	2830	rBV2	311	263	0.02%	0.003%
69	10.468	2836	2839	2842	rBV	269	198	0.02%	0.002%
70	10.674	2895	2903	2910	rVB4	2495	3331	0.28%	0.034%
71	10.758	2916	2929	2948	rBV	424585	687661	57.54%	6.969%
72	10.877	2962	2966	2968	rBV2	446	414	0.03%	0.004%
73	10.893	2968	2971	2979	rVB5	1280	1595	0.13%	0.016%
74	10.970	2993	2995	3000	rVB2	290	184	0.02%	0.002%
75	11.005	3004	3006	3009	rBV2	277	188	0.02%	0.002%
76	11.118	3038	3041	3043	rBV	570	268	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048133.D
 Acq On : 19 Apr 2022 15:12
 Operator : SY/MD
 Sample : N2419-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.439	3137	3141	3142	rBV2	416	231	0.02%	0.002%
78	11.459	3142	3147	3159	rVB4	1420	2349	0.20%	0.024%
79	11.584	3183	3186	3189	rBV	443	304	0.03%	0.003%
80	11.696	3213	3221	3227	rBV3	793	1213	0.10%	0.012%
81	11.751	3234	3238	3242	rVB	584	476	0.04%	0.005%
82	11.815	3242	3258	3278	rBV	661279	1059764	88.67%	10.740%
83	11.973	3303	3307	3315	rVB5	1893	2312	0.19%	0.023%
84	12.066	3332	3336	3337	rBV	832	557	0.05%	0.006%
85	12.195	3362	3376	3403	rBV	570723	925196	77.41%	9.376%
86	12.333	3412	3419	3423	rBV4	755	957	0.08%	0.010%
87	12.401	3436	3440	3444	rBV4	387	368	0.03%	0.004%
88	12.526	3477	3479	3482	rVB	377	192	0.02%	0.002%
89	12.545	3482	3485	3490	rBV2	466	480	0.04%	0.005%
90	12.639	3511	3514	3515	rBV2	354	181	0.02%	0.002%
91	12.915	3597	3600	3603	rBV3	367	323	0.03%	0.003%
92	13.095	3652	3656	3659	rBV2	347	273	0.02%	0.003%
93	13.233	3693	3699	3704	rBV4	716	1091	0.09%	0.011%
94	13.413	3753	3755	3757	rBV2	303	179	0.01%	0.002%
95	13.581	3804	3807	3809	rBV2	277	228	0.02%	0.002%
96	13.626	3819	3821	3827	rBV2	252	241	0.02%	0.002%
97	13.658	3828	3831	3836	rVV2	292	253	0.02%	0.003%
98	13.851	3883	3891	3899	rBV4	1832	2389	0.20%	0.024%
99	14.098	3963	3968	3976	rVB3	1565	2067	0.17%	0.021%
100	14.330	4035	4040	4049	rBV3	1432	2072	0.17%	0.021%




Sum of corrected areas: 9867876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048133.D
Acq On : 19 Apr 2022 15:12
Operator : SY/MD
Sample : N2419-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

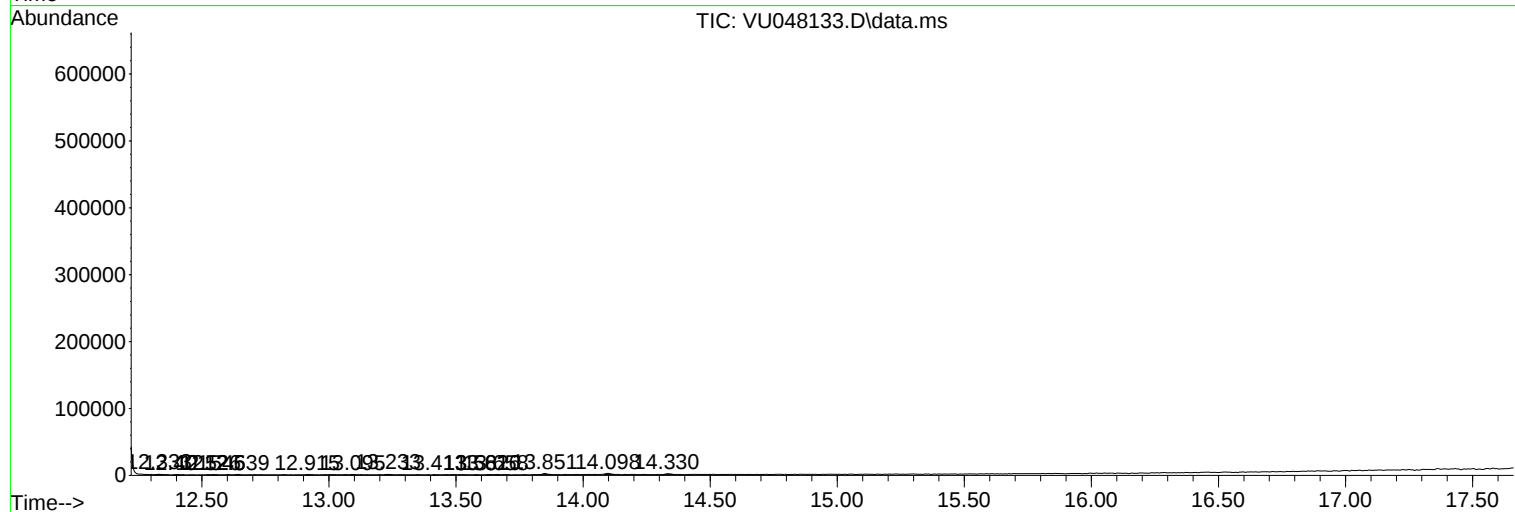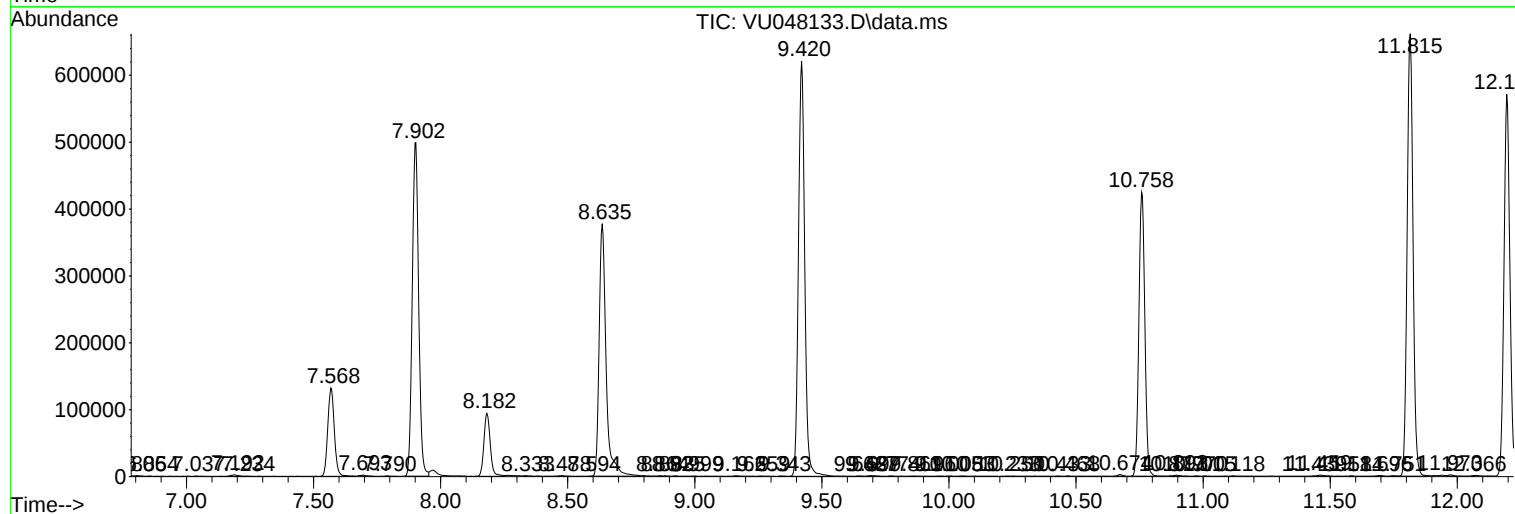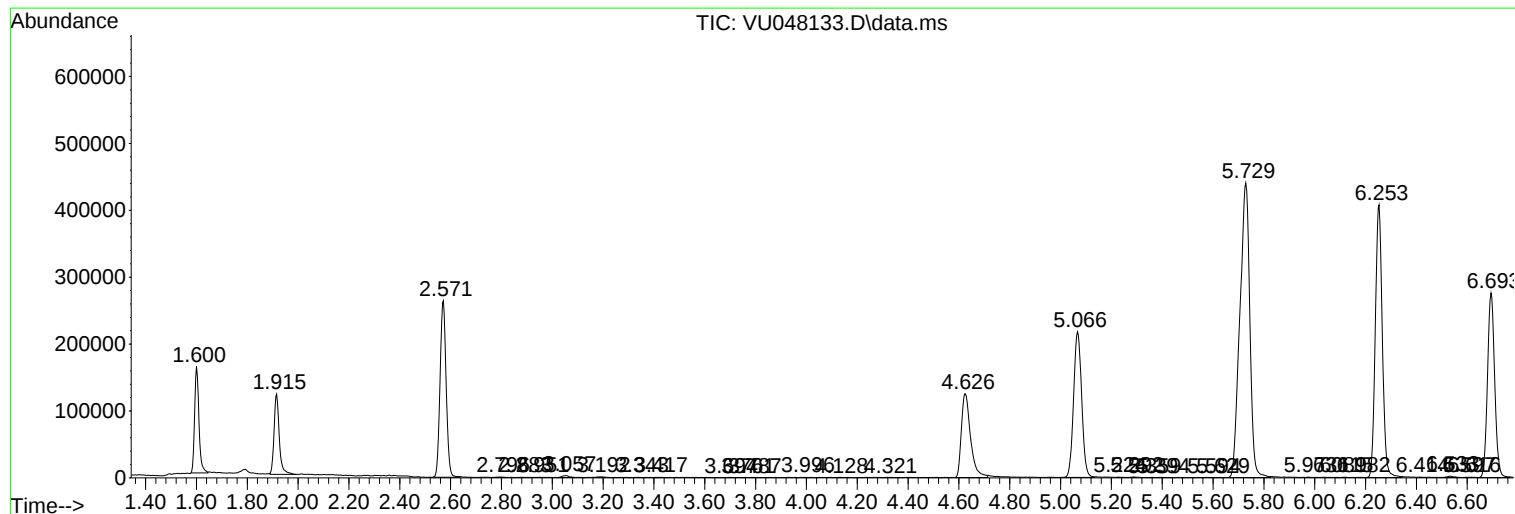

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048133.D
Acq On : 19 Apr 2022 15:12
Operator : SY/MD
Sample : N2419-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048133.D
Acq On : 19 Apr 2022 15:12
Operator : SY/MD
Sample : N2419-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------