

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048135.D
 Acq On : 19 Apr 2022 16:37
 Operator : SY/MD
 Sample : N2419-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	101	rBV	173640	208124	15.68%	2.015%
2	1.916	171	179	195	rBV	134039	183246	13.81%	1.774%
3	2.443	340	343	346	rBV2	421	268	0.02%	0.003%
4	2.488	355	357	364	rVB3	229	204	0.02%	0.002%
5	2.571	370	383	404	rBV	281006	476000	35.87%	4.608%
6	2.726	429	431	433	rBV	299	163	0.01%	0.002%
7	2.835	460	465	467	rBV2	244	245	0.02%	0.002%
8	2.883	477	480	486	rBV2	377	460	0.03%	0.004%
9	2.954	498	502	503	rBV	289	196	0.01%	0.002%
10	3.006	516	518	524	rVV2	257	179	0.01%	0.002%
11	3.051	524	532	541	rVV3	1978	3337	0.25%	0.032%
12	3.189	562	575	590	rVB2	6269	14013	1.06%	0.136%
13	3.353	622	626	630	rVB2	297	229	0.02%	0.002%
14	3.588	693	699	704	rVV2	193	241	0.02%	0.002%
15	3.957	809	814	817	rBV2	220	195	0.01%	0.002%
16	4.189	881	886	891	rBV2	177	207	0.02%	0.002%
17	4.247	901	904	912	rVB2	190	223	0.02%	0.002%
18	4.333	928	931	937	rVB2	177	190	0.01%	0.002%
19	4.427	955	960	963	rBV2	241	176	0.01%	0.002%
20	4.559	998	1001	1004	rBV2	340	290	0.02%	0.003%
21	4.636	1010	1025	1055	rBV	136534	380841	28.70%	3.687%
22	4.890	1101	1104	1106	rBV3	260	195	0.01%	0.002%
23	4.903	1106	1108	1112	rVB	434	255	0.02%	0.002%
24	4.925	1112	1115	1120	rBV3	308	282	0.02%	0.003%
25	4.983	1130	1133	1136	rBV	278	160	0.01%	0.002%
26	5.067	1141	1159	1189	rVV	241662	527441	39.74%	5.106%
27	5.243	1213	1214	1221	rVB	246	186	0.01%	0.002%
28	5.295	1221	1230	1236	rVB4	544	1038	0.08%	0.010%
29	5.394	1258	1261	1268	rBV	149	206	0.02%	0.002%
30	5.552	1306	1310	1314	rBV2	241	267	0.02%	0.003%
31	5.729	1336	1365	1397	rBV2	491405	1327126	100.00%	12.847%
32	6.012	1448	1453	1458	rBV3	221	269	0.02%	0.003%
33	6.038	1458	1461	1464	rBV2	264	196	0.01%	0.002%
34	6.121	1482	1487	1491	rBV3	463	393	0.03%	0.004%
35	6.163	1497	1500	1506	rVB2	307	317	0.02%	0.003%
36	6.253	1511	1528	1549	rBV	382827	736507	55.50%	7.130%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048135.D
 Acq On : 19 Apr 2022 16:37
 Operator : SY/MD
 Sample : N2419-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.423	1577	1581	1589	rVB4	427	528	0.04%	0.005%
38	6.530	1607	1614	1629	rVB5	2346	4303	0.32%	0.042%
39	6.693	1647	1665	1689	rBV	302374	596453	44.94%	5.774%
40	6.816	1698	1703	1708	rVB4	943	1219	0.09%	0.012%
41	6.947	1740	1744	1748	rVB2	213	170	0.01%	0.002%
42	6.976	1749	1753	1756	rBV	327	259	0.02%	0.003%
43	7.054	1770	1777	1784	rVB2	617	791	0.06%	0.008%
44	7.192	1809	1820	1830	rBV5	2562	4751	0.36%	0.046%
45	7.346	1865	1868	1872	rVB2	266	193	0.01%	0.002%
46	7.388	1878	1881	1884	rBV	189	161	0.01%	0.002%
47	7.472	1902	1907	1909	rBV	188	167	0.01%	0.002%
48	7.501	1913	1916	1921	rVB	279	214	0.02%	0.002%
49	7.568	1921	1937	1956	rBV	144232	254668	19.19%	2.465%
50	7.690	1969	1975	1977	rBV3	1263	1328	0.10%	0.013%
51	7.735	1987	1989	1992	rVB2	294	173	0.01%	0.002%
52	7.793	2003	2007	2008	rBV	391	227	0.02%	0.002%
53	7.819	2013	2015	2019	rVB	442	248	0.02%	0.002%
54	7.899	2019	2040	2057	rBV	559305	983566	74.11%	9.521%
55	8.182	2116	2128	2149	rBV	107197	187453	14.12%	1.815%
56	8.475	2210	2219	2226	rVB3	715	1388	0.10%	0.013%
57	8.520	2231	2233	2236	rBV	305	202	0.02%	0.002%
58	8.639	2256	2270	2316	rBV	403756	783932	59.07%	7.589%
59	9.073	2399	2405	2407	rBV2	212	186	0.01%	0.002%
60	9.089	2407	2410	2413	rVV2	295	256	0.02%	0.002%
61	9.160	2429	2432	2437	rVV3	362	322	0.02%	0.003%
62	9.253	2457	2461	2466	rVB3	266	255	0.02%	0.002%
63	9.349	2484	2491	2495	rVB2	344	360	0.03%	0.003%
64	9.420	2495	2513	2552	rBV	581160	991270	74.69%	9.596%
65	9.568	2556	2559	2561	rBV2	319	221	0.02%	0.002%
66	9.607	2568	2571	2574	rBV2	361	243	0.02%	0.002%
67	9.639	2579	2581	2584	rBV	392	218	0.02%	0.002%
68	9.655	2584	2586	2589	rVB2	398	203	0.02%	0.002%
69	9.700	2593	2600	2605	rVB	736	905	0.07%	0.009%
70	9.754	2609	2617	2621	rBV2	346	424	0.03%	0.004%
71	9.931	2670	2672	2677	rVB2	329	222	0.02%	0.002%
72	10.674	2896	2903	2910	rBV3	3213	4003	0.30%	0.039%
73	10.758	2917	2929	2951	rVB	467589	747123	56.30%	7.233%
74	10.835	2951	2953	2956	rVB	350	162	0.01%	0.002%
75	10.873	2956	2965	2967	rBV4	608	774	0.06%	0.007%
76	10.973	2992	2996	2997	rBV	392	205	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048135.D
 Acq On : 19 Apr 2022 16:37
 Operator : SY/MD
 Sample : N2419-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.018	3007	3010	3014	rVB2	322	251	0.02%	0.002%
78	11.050	3014	3020	3023	rBV2	248	262	0.02%	0.003%
79	11.118	3037	3041	3045	rBV3	646	470	0.04%	0.005%
80	11.205	3065	3068	3070	rVB	422	167	0.01%	0.002%
81	11.224	3070	3074	3077	rBV	280	223	0.02%	0.002%
82	11.291	3092	3095	3098	rBV	293	187	0.01%	0.002%
83	11.381	3119	3123	3125	rBV	272	184	0.01%	0.002%
84	11.401	3126	3129	3134	rVV2	183	165	0.01%	0.002%
85	11.462	3140	3148	3160	rVB9	1471	2670	0.20%	0.026%
86	11.578	3181	3184	3195	rBV2	503	642	0.05%	0.006%
87	11.697	3213	3221	3227	rVB5	909	1096	0.08%	0.011%
88	11.742	3233	3235	3241	rVB2	514	325	0.02%	0.003%
89	11.815	3245	3258	3280	rBV	573983	923404	69.58%	8.939%
90	11.970	3302	3306	3315	rVB5	1548	1966	0.15%	0.019%
91	12.021	3319	3322	3327	rVB2	328	284	0.02%	0.003%
92	12.076	3336	3339	3346	rVB3	356	374	0.03%	0.004%
93	12.114	3346	3351	3355	rBV2	358	359	0.03%	0.003%
94	12.195	3362	3376	3399	rBV	582801	960997	72.41%	9.303%
95	12.484	3462	3466	3471	rBV	368	348	0.03%	0.003%
96	12.536	3478	3482	3486	rBV2	364	338	0.03%	0.003%
97	12.616	3504	3507	3512	rBV2	458	310	0.02%	0.003%
98	13.905	3904	3908	3911	rBV3	618	563	0.04%	0.005%
99	14.548	4105	4108	4110	rBV	536	355	0.03%	0.003%
100	15.085	4273	4275	4281	rBV4	462	425	0.03%	0.004%




Sum of corrected areas: 10329976

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048135.D
Acq On : 19 Apr 2022 16:37
Operator : SY/MD
Sample : N2419-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

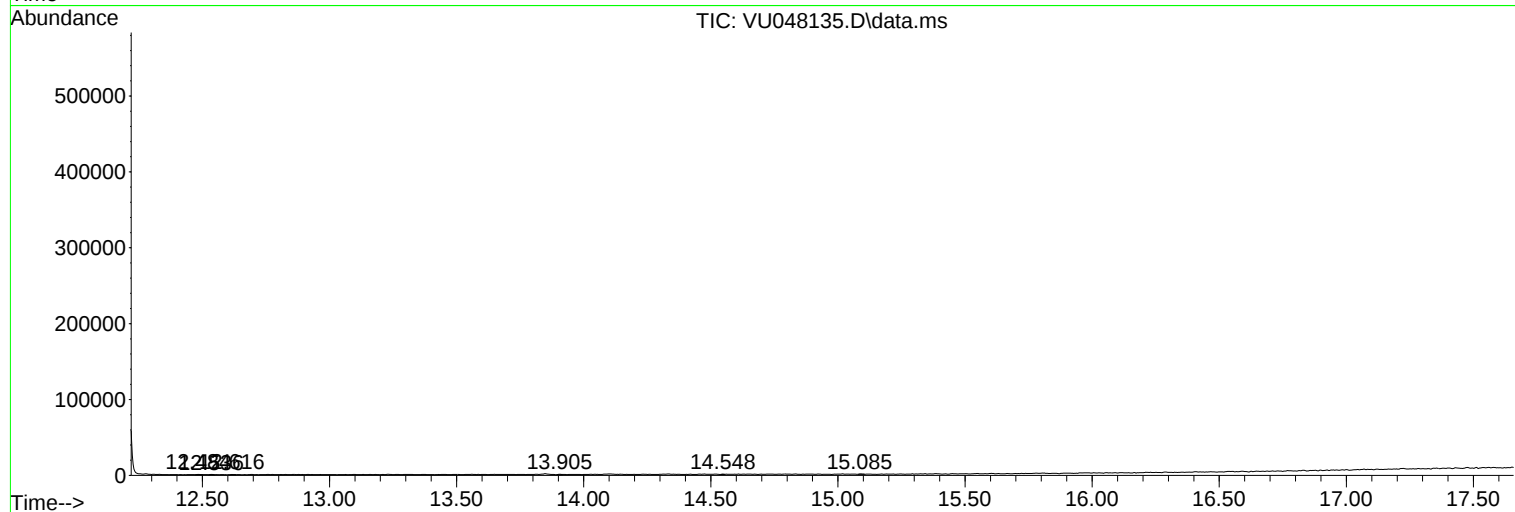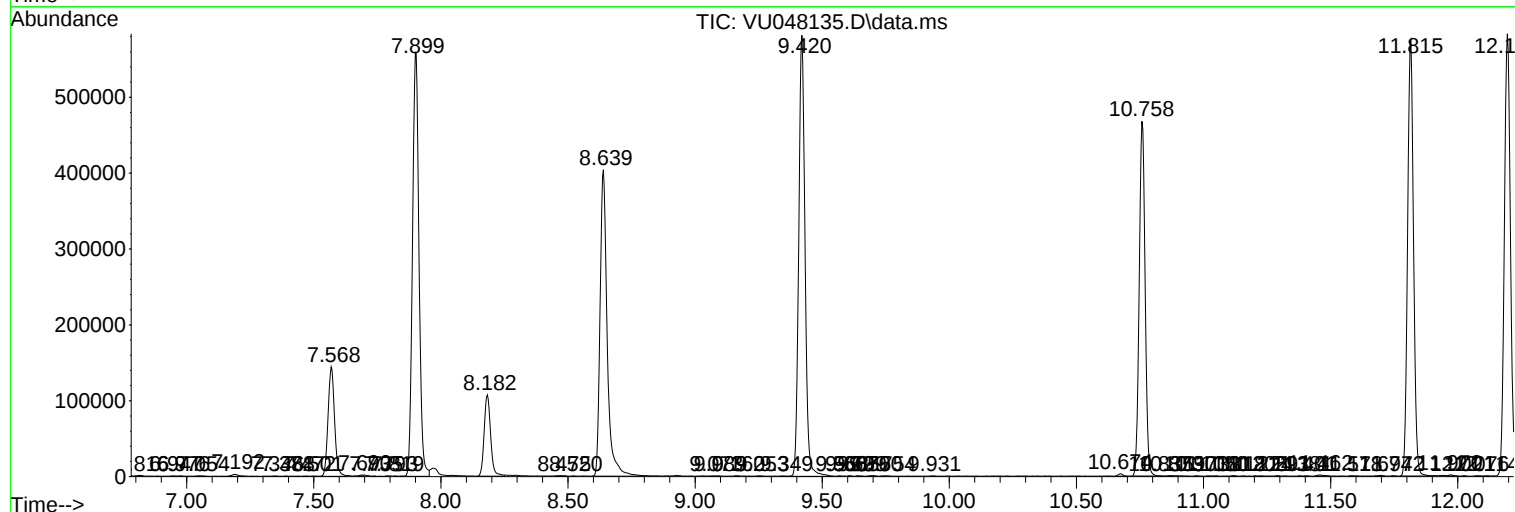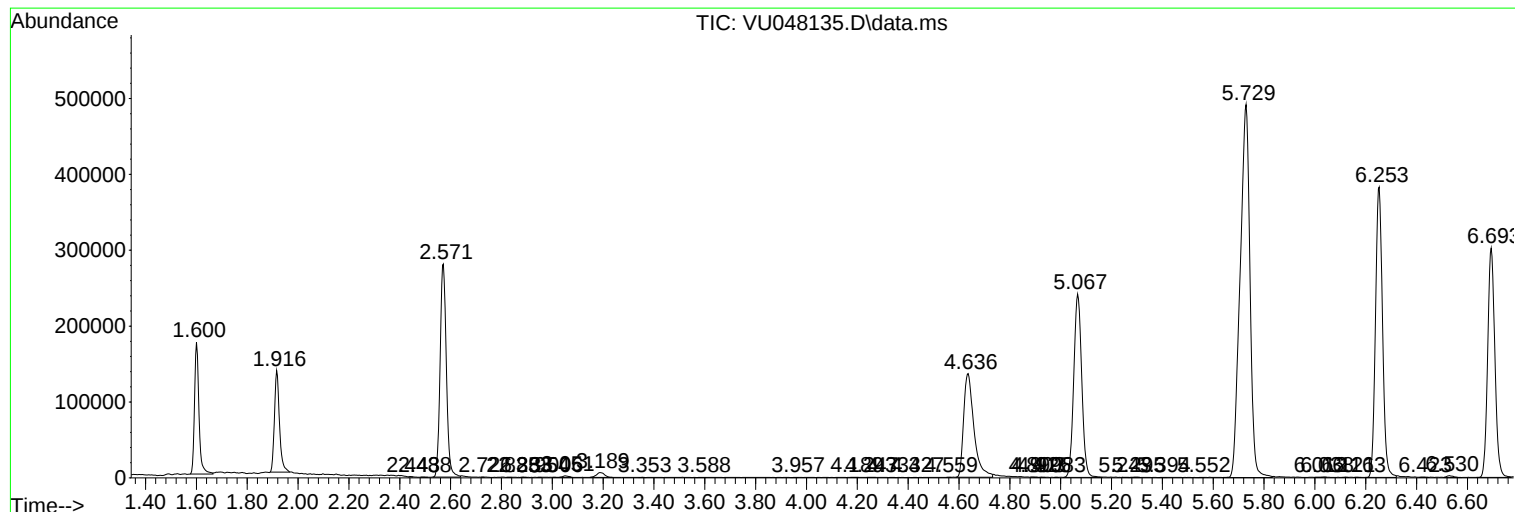

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048135.D
Acq On : 19 Apr 2022 16:37
Operator : SY/MD
Sample : N2419-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
Data File : VU048135.D
Acq On : 19 Apr 2022 16:37
Operator : SY/MD
Sample : N2419-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------