
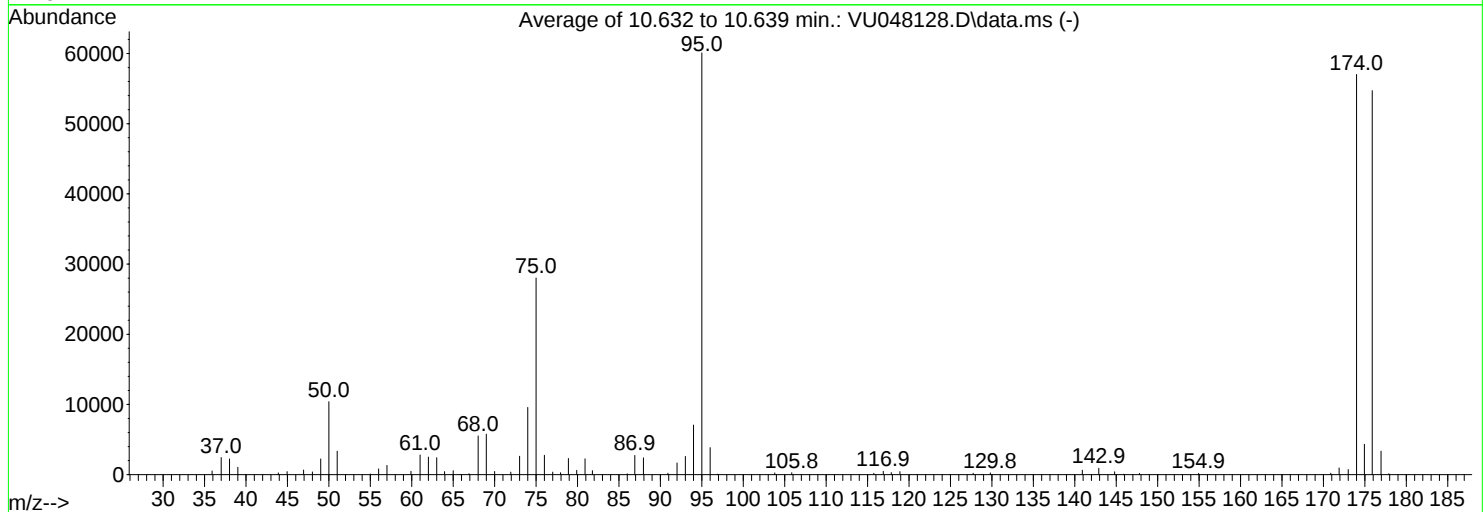


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041922\
 Data File : VU048128.D
 Acq On : 19 Apr 2022 09:02
 Operator : SY/MD
 Sample : BFB067
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB067

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 22 02:51:38 2022

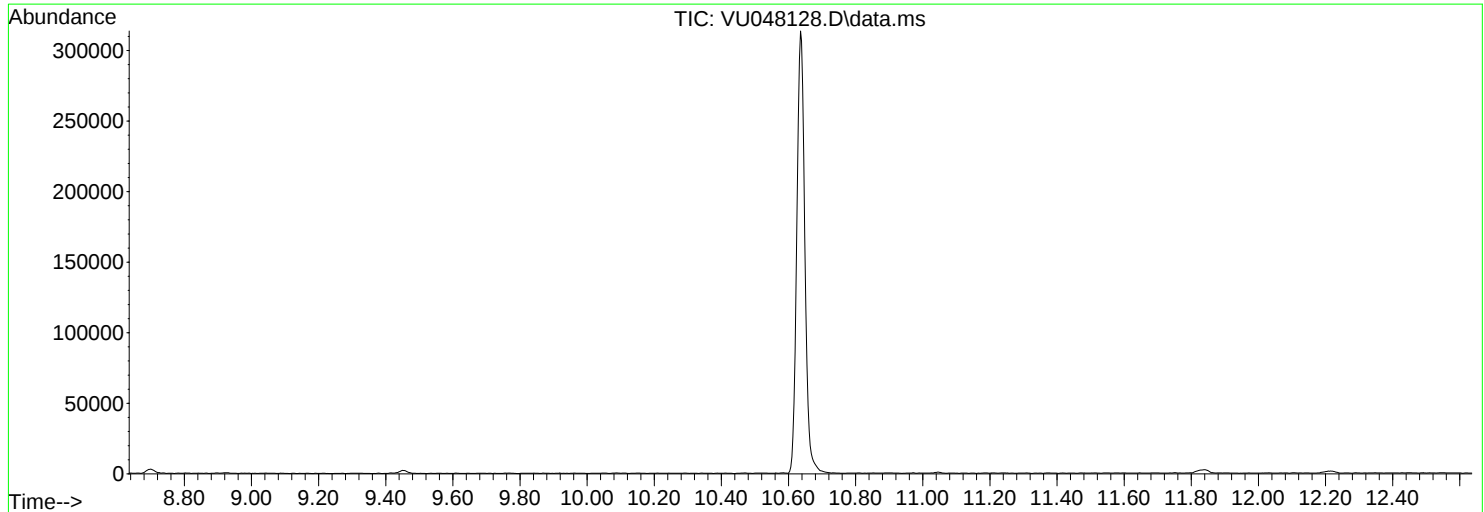

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	10400	PASS
75	95	30	80	46.6	28011	PASS
95	95	100	100	100.0	60091	PASS
96	95	5	9	6.4	3857	PASS
173	174	0.00	2	1.3	720	PASS
174	95	50	120	94.9	57008	PASS
175	174	5	9	7.6	4324	PASS
176	174	95	101	96.0	54707	PASS
177	176	5	9	6.1	3350	PASS

m/z	Abundance
35.90	548.0
37.00	2501.0
38.00	2273.0
39.00	1085.0
40.00	193.0
43.90	689.0
44.90	457.0
46.90	711.0
48.00	405.0
49.00	2303.0
50.00	10709.0
51.00	3469.0
55.00	144.0
56.00	857.0
57.00	1369.0
59.90	482.0
61.00	2938.0
62.00	2555.0
63.00	2489.0
63.90	445.0
65.00	583.0
66.90	144.0
68.00	5643.0
69.00	5886.0
70.00	486.0
71.90	391.0
73.00	2738.0
74.00	9839.0
75.00	28768.0
76.00	2828.0
77.00	378.0
77.90	265.0
78.90	2370.0
79.90	610.0
80.90	2317.0
81.80	592.0
86.00	114.0
86.90	2860.0
87.90	2470.0
90.90	214.0
92.00	1715.0
93.00	2699.0
94.00	7228.0
95.00	61824.0
96.00	3871.0
96.90	103.0
103.80	255.0
105.90	292.0
115.80	205.0
116.90	480.0
117.80	290.0
118.90	435.0
127.70	218.0
129.80	255.0
140.90	667.0
142.90	963.0
144.80	424.0
145.90	116.0
147.80	194.0
154.90	180.0
170.90	210.0
171.90	995.0
173.00	744.0
174.00	58824.0
174.90	4463.0
175.90	56416.0
176.90	3447.0
177.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
40.00	161.0
44.00	405.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	520.0
37.00	2392.0
38.00	2243.0
39.00	1003.0
39.90	225.0
43.90	621.0
45.00	427.0
46.90	622.0
48.00	367.0
49.00	2307.0
50.00	10215.0
51.00	3307.0
56.00	834.0
57.00	1262.0
59.90	448.0
61.00	2587.0
62.00	2466.0
63.00	2415.0
64.00	484.0
65.00	513.0
66.90	194.0
68.00	5663.0
69.00	5720.0
70.00	475.0
72.00	350.0
73.00	2495.0
74.00	9271.0
75.00	27560.0
76.00	2693.0
77.00	308.0
78.00	272.0
78.90	2259.0
79.90	575.0
80.90	2183.0
81.80	528.0
86.00	108.0
86.90	2694.0
87.90	2356.0
90.90	191.0
92.00	1675.0
93.00	2489.0
94.00	6975.0
95.00	57712.0
96.00	3878.0
103.70	246.0
105.80	283.0
115.80	194.0
116.90	495.0
117.90	280.0
118.90	401.0
127.80	186.0
129.80	252.0
140.90	636.0
142.90	879.0
144.80	378.0
147.80	158.0
155.00	159.0
170.90	180.0
171.90	875.0
173.00	723.0
174.00	54048.0
174.90	4216.0
175.90	51776.0
176.90	3234.0
177.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	502.0
37.00	2435.0
38.00	2165.0
39.00	1065.0
40.00	176.0
43.90	660.0
44.90	452.0
47.00	676.0
48.00	383.0
49.00	2125.0
50.00	10275.0
51.00	3306.0
55.00	166.0
56.00	782.0
57.00	1363.0
59.90	489.0
61.00	2884.0
62.00	2495.0
63.00	2342.0
63.90	359.0
65.00	637.0
65.80	106.0
66.90	110.0
68.00	5264.0
69.00	5669.0
70.00	406.0
71.90	370.0
73.00	2625.0
74.00	9627.0
75.00	27704.0
76.00	2738.0
77.00	418.0
77.90	254.0
78.90	2293.0
79.90	669.0
80.90	2274.0
81.80	596.0
86.00	131.0
86.90	2662.0
88.00	2368.0
90.90	205.0
92.00	1630.0
93.00	2625.0
94.00	6984.0
95.00	60736.0
96.00	3822.0
96.90	126.0
103.90	251.0
105.90	281.0
115.70	194.0
116.90	459.0
117.80	292.0
118.90	474.0
127.70	233.0
128.80	112.0
129.80	229.0
140.90	604.0
142.90	917.0
144.80	431.0
145.90	127.0
147.80	177.0
154.90	231.0
170.90	201.0
171.90	1007.0
173.00	692.0
174.00	58152.0
175.00	4294.0
175.90	55928.0
177.00	3369.0
177.90	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067