


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042019\
 Data File : VU031353.D
 Acq On : 19 Apr 2019 12:44
 Operator : JC/SP
 Sample : BFB59
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB59

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM041719WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 23 02:53:18 2019

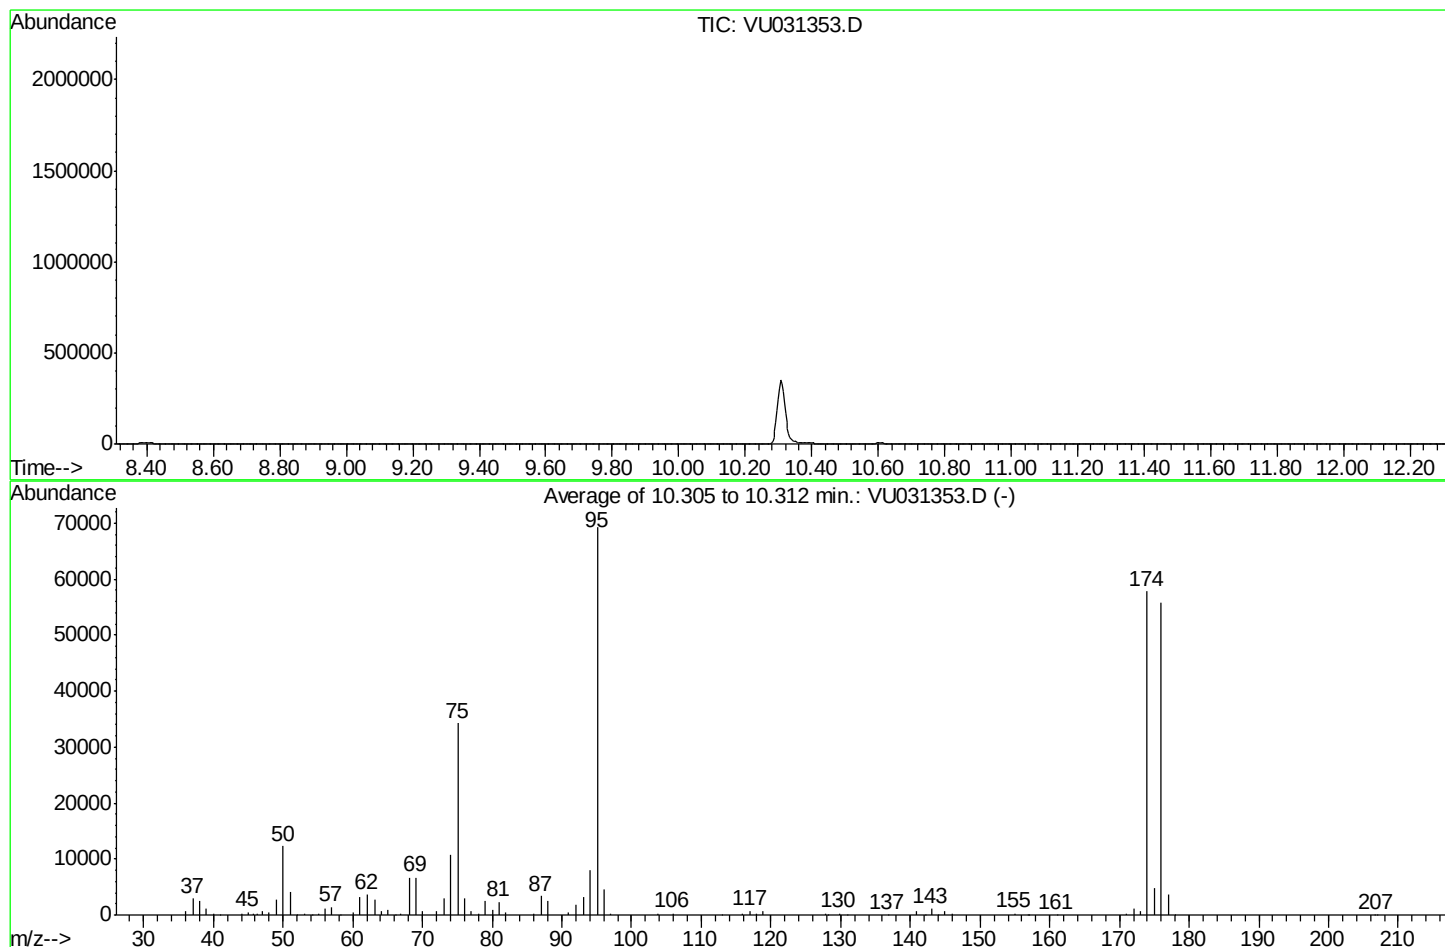

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	12325	PASS
75	95	30	80	49.5	34269	PASS
95	95	100	100	100.0	69234	PASS
96	95	5	9	6.8	4694	PASS
173	174	0.00	2	1.2	670	PASS
174	95	50	120	83.4	57752	PASS
175	174	5	9	8.2	4730	PASS
176	174	95	101	96.8	55898	PASS
177	176	5	9	6.7	3726	PASS

Scan 2854 (10.267 min): VU031353.D
BFB59

m/z	Abundance
40.00	766.0
43.10	184.0
44.10	791.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.10	722.0
37.10	3130.0
38.00	2763.0
39.00	1334.0
40.00	994.0
41.00	106.0
44.00	1125.0
44.90	448.0
45.70	246.0
46.30	265.0
46.90	646.0
48.00	373.0
49.00	2915.0
50.00	12242.0
51.10	4248.0
52.00	153.0
53.10	303.0
55.00	144.0
56.00	1241.0
57.00	1651.0
58.10	116.0
60.00	513.0
61.10	3006.0
62.00	3510.0
63.10	2871.0
64.10	775.0
65.00	717.0
66.90	120.0
68.10	7112.0
69.00	6931.0
70.00	734.0
72.10	684.0
73.10	2801.0
74.00	10744.0
75.10	35016.0
76.10	3053.0
76.90	591.0
78.10	283.0
79.00	2485.0
80.00	862.0
81.00	2437.0
81.90	489.0
87.00	3586.0
88.00	2652.0
90.90	464.0
92.10	1710.0
93.10	3122.0
94.10	8218.0
95.10	68896.0
96.10	4768.0
97.00	157.0
103.70	237.0
105.90	370.0
116.00	197.0
117.00	772.0
117.90	225.0
118.80	569.0
127.80	232.0
128.20	160.0
129.80	207.0
131.00	123.0
136.80	150.0
140.90	610.0
143.00	1047.0
144.90	622.0
146.00	165.0
155.00	310.0
156.80	206.0
170.90	237.0
172.00	1049.0
173.00	1061.0
174.00	56000.0
175.10	4757.0
176.00	54912.0
177.10	3386.0
177.90	102.0
206.70	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.10	766.0
37.10	2947.0
38.00	2505.0
38.90	1153.0
40.00	988.0
44.00	1005.0
45.00	518.0
45.70	158.0
46.30	122.0
47.00	714.0
48.00	371.0
49.10	2798.0
50.00	12769.0
51.10	4313.0
52.00	110.0
53.10	204.0
54.10	104.0
55.10	173.0
56.00	1259.0
57.00	1447.0
58.20	115.0
60.00	501.0
61.00	3250.0
62.10	3675.0
63.10	2945.0
64.10	788.0
65.10	876.0
66.80	169.0
68.10	6689.0
69.00	6772.0
70.00	683.0
72.00	754.0
73.00	2952.0
74.00	10994.0
75.10	35304.0
76.10	3078.0
77.00	748.0
78.10	272.0
79.00	2540.0
80.00	868.0
81.00	2345.0
81.90	500.0
85.90	155.0
87.00	3608.0
88.00	2559.0
90.90	453.0
92.10	1833.0
93.10	3261.0
94.10	8031.0
95.10	71304.0
96.10	4824.0
96.90	144.0
103.70	253.0
105.90	290.0
116.00	240.0
117.00	751.0
118.00	278.0
118.90	724.0
127.70	217.0
129.80	243.0
136.80	150.0
140.90	592.0
142.20	127.0
143.00	1162.0
144.00	130.0
144.90	767.0
146.00	191.0
155.00	267.0
157.00	170.0
161.00	120.0
171.00	272.0
172.00	1139.0
173.00	950.0
174.00	59304.0
175.00	4842.0
176.00	57808.0
177.10	3782.0
206.70	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59

m/z	Abundance
36.10	744.0
37.10	2633.0
38.10	2253.0
38.90	910.0
40.00	925.0
44.10	950.0
45.00	476.0
45.80	118.0
47.00	811.0
47.90	459.0
49.10	2583.0
50.00	11965.0
51.10	3791.0
53.00	112.0
55.10	217.0
56.00	1173.0
56.90	1250.0
60.00	552.0
61.00	3307.0
62.10	3573.0
63.10	2553.0
64.00	717.0
65.10	923.0
66.20	107.0
66.80	219.0
68.10	5968.0
69.00	6333.0
70.00	486.0
71.90	668.0
73.00	2965.0
74.00	10305.0
75.10	32488.0
76.00	2768.0
77.00	828.0
78.10	276.0
79.00	2355.0
80.00	710.0
80.90	2136.0
81.90	496.0
85.90	220.0
87.00	3061.0
88.10	2423.0
90.90	381.0
92.10	1829.0
93.10	3099.0
94.10	7652.0
95.10	67504.0
96.10	4490.0
96.90	183.0
103.70	211.0
105.90	167.0
113.00	107.0
115.90	212.0
117.10	650.0
118.00	241.0
118.90	676.0
127.80	232.0
129.90	260.0
140.90	629.0
142.20	113.0
143.00	1215.0
144.00	166.0
145.00	807.0
146.00	116.0
154.90	178.0
157.00	186.0
161.00	125.0
171.10	257.0
172.00	1157.0
174.00	57952.0
175.00	4592.0
176.00	54976.0
177.00	4010.0
206.90	258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB59