


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU042020\
Data File : VU037804.D
Acq On : 20 Apr 2020 09:14
Operator : JC/MD
Sample : BFB17
Misc : 25mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB17

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Apr 21 01:10:29 2020

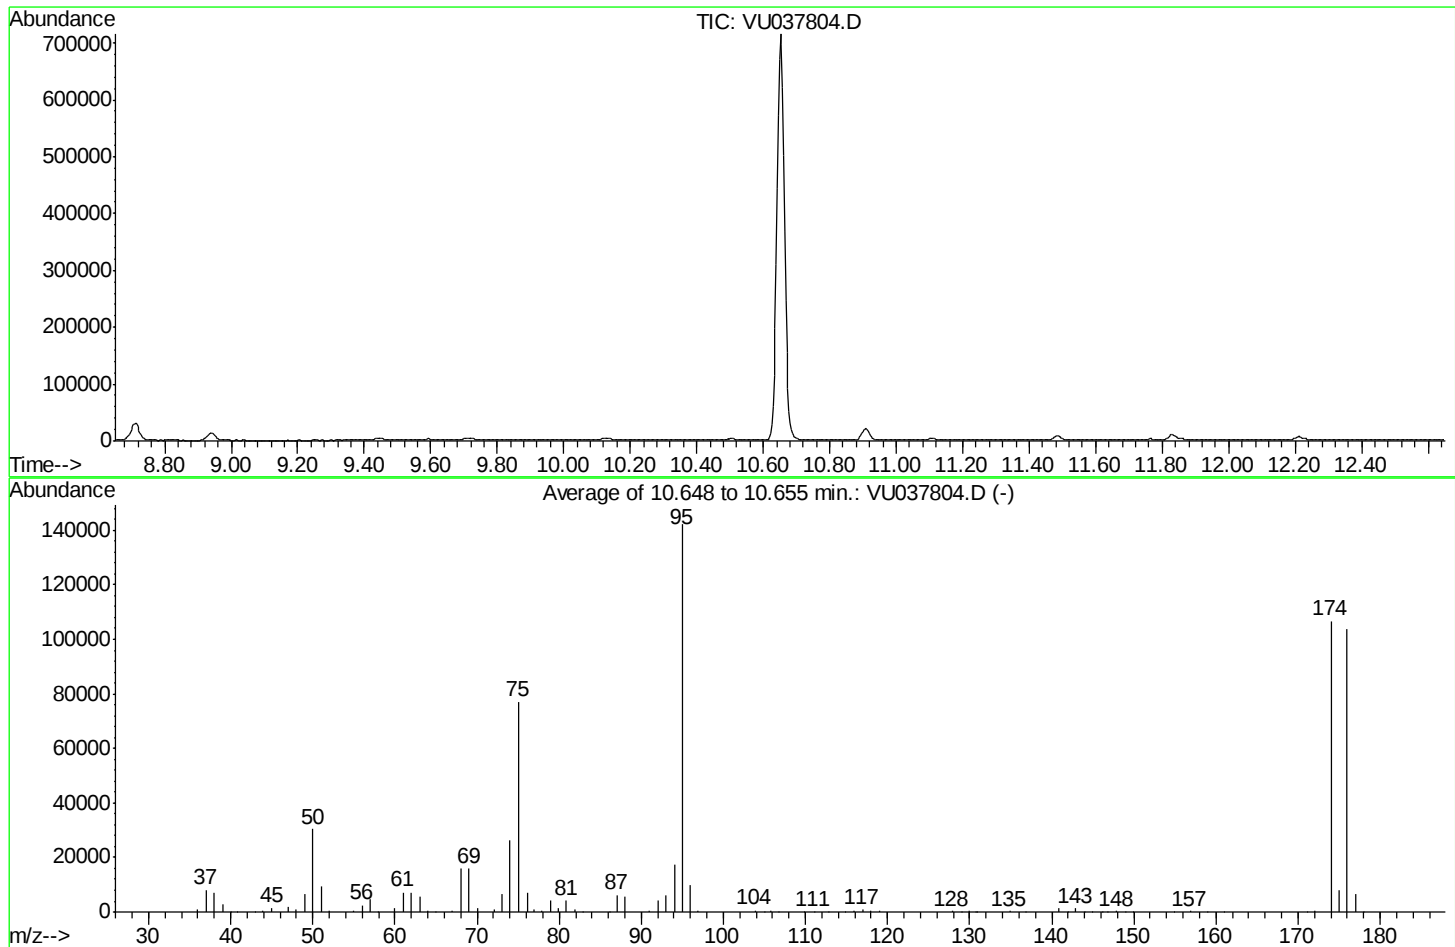

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	30413	PASS
75	95	30	80	54.2	77082	PASS
95	95	100	100	100.0	142186	PASS
96	95	5	9	6.9	9742	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	106765	PASS
175	174	5	9	7.4	7888	PASS
176	174	95	101	97.2	103765	PASS
177	176	5	9	6.2	6460	PASS

m/z	Abundance
36.00	1930.0
37.00	7938.0
38.00	7054.0
39.00	2676.0
40.00	203.0
40.80	100.0
43.00	206.0
44.00	1429.0
45.00	1545.0
47.00	2095.0
47.90	861.0
49.00	6266.0
50.00	29632.0
51.00	9521.0
52.00	468.0
55.10	402.0
56.00	2369.0
57.00	4454.0
57.80	174.0
59.90	1502.0
61.00	6961.0
62.00	6692.0
63.00	5833.0
64.00	573.0
65.00	106.0
67.00	533.0
68.00	15782.0
69.00	15445.0
70.10	1260.0
72.10	923.0
73.00	6700.0
74.00	26184.0
75.00	74168.0
76.10	6944.0
77.00	885.0
77.90	589.0
78.90	4259.0
80.00	1059.0
80.90	4071.0
81.90	870.0
82.90	130.0
86.10	204.0
87.00	5673.0
88.00	5541.0
90.90	628.0
92.00	4253.0
93.00	5944.0
94.10	16464.0
95.00	138560.0
96.00	9745.0
97.00	368.0
103.90	616.0
105.00	204.0
105.80	542.0
106.70	135.0
111.00	117.0
112.90	109.0
114.80	250.0
115.90	514.0
117.00	748.0
117.90	498.0
119.00	755.0
127.90	428.0
129.00	276.0
129.90	475.0
130.70	180.0
134.90	256.0
136.80	238.0
140.90	1128.0
141.90	128.0
142.90	1204.0
144.80	112.0
146.10	134.0
146.80	130.0
148.00	306.0
155.00	202.0
156.90	247.0
158.90	114.0
160.90	220.0
172.10	294.0
174.00	101224.0
175.00	7515.0
176.00	97080.0
177.00	6316.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
36.00	1898.0
37.00	8325.0
38.00	7215.0
39.00	2875.0
40.00	197.0
43.00	194.0
44.00	1491.0
45.00	1592.0
47.00	2051.0
47.90	879.0
49.00	6560.0
50.00	31352.0
51.00	9894.0
52.00	467.0
54.90	496.0
56.00	2517.0
57.00	4727.0
57.90	204.0
59.90	1513.0
61.00	7423.0
62.00	7088.0
63.00	5736.0
64.00	683.0
65.00	118.0
67.00	526.0
68.00	16138.0
69.00	16137.0
70.10	1243.0
72.10	1014.0
73.00	6779.0
74.00	27096.0
75.00	79368.0
76.10	7125.0
77.00	867.0
77.80	709.0
78.90	4375.0
79.90	1274.0
80.90	4138.0
81.90	910.0
82.80	107.0
87.00	6296.0
88.00	6103.0
90.90	727.0
92.00	4456.0
93.00	6425.0
94.00	17896.0
95.00	146432.0
96.00	9916.0
97.00	349.0
103.90	607.0
104.90	155.0
105.80	587.0
106.80	145.0
109.80	103.0
111.00	125.0
112.80	127.0
114.90	221.0
115.90	507.0
117.00	875.0
117.90	563.0
119.00	758.0
127.90	463.0
129.00	253.0
129.90	456.0
130.90	228.0
134.90	307.0
136.90	256.0
140.90	1229.0
142.00	132.0
142.90	1390.0
143.90	100.0
144.80	118.0
146.10	129.0
146.80	115.0
148.00	334.0
149.00	114.0
149.90	130.0
155.00	244.0
156.90	284.0
158.90	115.0
160.90	253.0
172.00	284.0
174.00	110008.0
175.00	8089.0
176.00	107264.0
177.00	6651.0
178.00	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
35.00	1763.0
37.00	7832.0
38.00	6986.0
39.00	2753.0
39.00	233.0
43.00	176.0
44.00	1501.0
45.00	1451.0
47.00	1879.0
48.00	772.0
49.00	6474.0
50.00	30256.0
51.00	9213.0
52.00	414.0
54.00	537.0
56.00	2448.0
57.00	4397.0
57.00	162.0
59.00	1318.0
61.00	7150.0
62.00	6913.0
63.00	5253.0
64.00	690.0
65.00	194.0
67.00	514.0
68.00	15441.0
69.00	15833.0
70.00	1120.0
72.10	968.0
73.00	6426.0
74.00	25768.0
75.00	77712.0
76.10	6469.0
77.00	834.0
77.80	736.0
78.90	4105.0
79.90	1368.0
80.90	3984.0
81.90	889.0
87.00	6365.0
88.00	5890.0
90.90	698.0
92.00	4100.0
93.00	6238.0
94.00	17920.0
95.00	141568.0
96.00	9565.0
96.90	264.0
103.90	576.0
105.10	109.0
105.80	585.0
106.70	157.0
109.80	115.0
111.10	129.0
112.80	117.0
114.90	179.0
115.90	444.0
117.00	943.0
117.90	594.0
119.00	640.0
127.90	466.0
129.00	236.0
129.90	422.0
131.00	267.0
134.90	273.0
136.90	248.0
140.90	1221.0
142.00	146.0
142.90	1436.0
144.00	105.0
144.90	118.0
146.10	123.0
147.90	315.0
149.00	151.0
149.90	185.0
154.90	272.0
156.90	254.0
158.90	103.0
160.90	239.0
171.10	105.0
172.00	253.0
174.00	109064.0
175.00	8060.0
176.00	106952.0
177.00	6414.0
178.00	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

Scan 2881 (10.603 min): VU037804.D
BFB17

m/z	Abundance
36.00	721.0
37.90	248.0
40.10	188.0
41.10	155.0
43.90	795.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17