

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
 Data File : VU043215.D
 Acq On : 20 Apr 2021 11:52
 Operator : SY/MD
 Sample : M2057-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4516

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	9	17	32	rBV	593387	609915	100.00%	17.249%
2	1.526	42	58	60	rBV5	5661	10804	1.77%	0.306%
3	1.604	75	82	104	rVB	30572	40041	6.57%	1.132%
4	1.919	172	180	193	rVB	26845	35296	5.79%	0.998%
5	2.575	373	384	403	rBV	64880	105898	17.36%	2.995%
6	3.054	524	533	545	rVB4	4101	7417	1.22%	0.210%
7	4.658	1016	1032	1075	rBV2	39957	159873	26.21%	4.521%
8	5.076	1147	1162	1182	rBV	63047	143950	23.60%	4.071%
9	5.735	1347	1367	1392	rVB3	116101	304324	49.90%	8.607%
10	6.259	1514	1530	1547	rBV2	109140	205034	33.62%	5.799%
11	6.552	1610	1621	1631	rVB4	6175	10324	1.69%	0.292%
12	6.703	1654	1668	1684	rBV	77590	150213	24.63%	4.248%
13	7.574	1927	1939	1954	rBV	39299	68566	11.24%	1.939%
14	7.909	2030	2043	2060	rBV	139849	239240	39.23%	6.766%
15	8.189	2118	2130	2144	rBV2	24978	42070	6.90%	1.190%
16	8.562	2235	2246	2259	rVB2	86758	142938	23.44%	4.043%
17	8.648	2259	2273	2307	rBV	198998	399847	65.56%	11.308%
18	9.426	2500	2515	2531	rBV	160707	264412	43.35%	7.478%
19	10.767	2921	2932	2947	rVB	59851	95855	15.72%	2.711%
20	11.822	3248	3260	3274	rBV	170408	263900	43.27%	7.464%
21	12.201	3366	3378	3396	rVB	148537	235933	38.68%	6.673%


Sum of corrected areas: 3535850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043215.D
Acq On : 20 Apr 2021 11:52
Operator : SY/MD
Sample : M2057-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4516

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

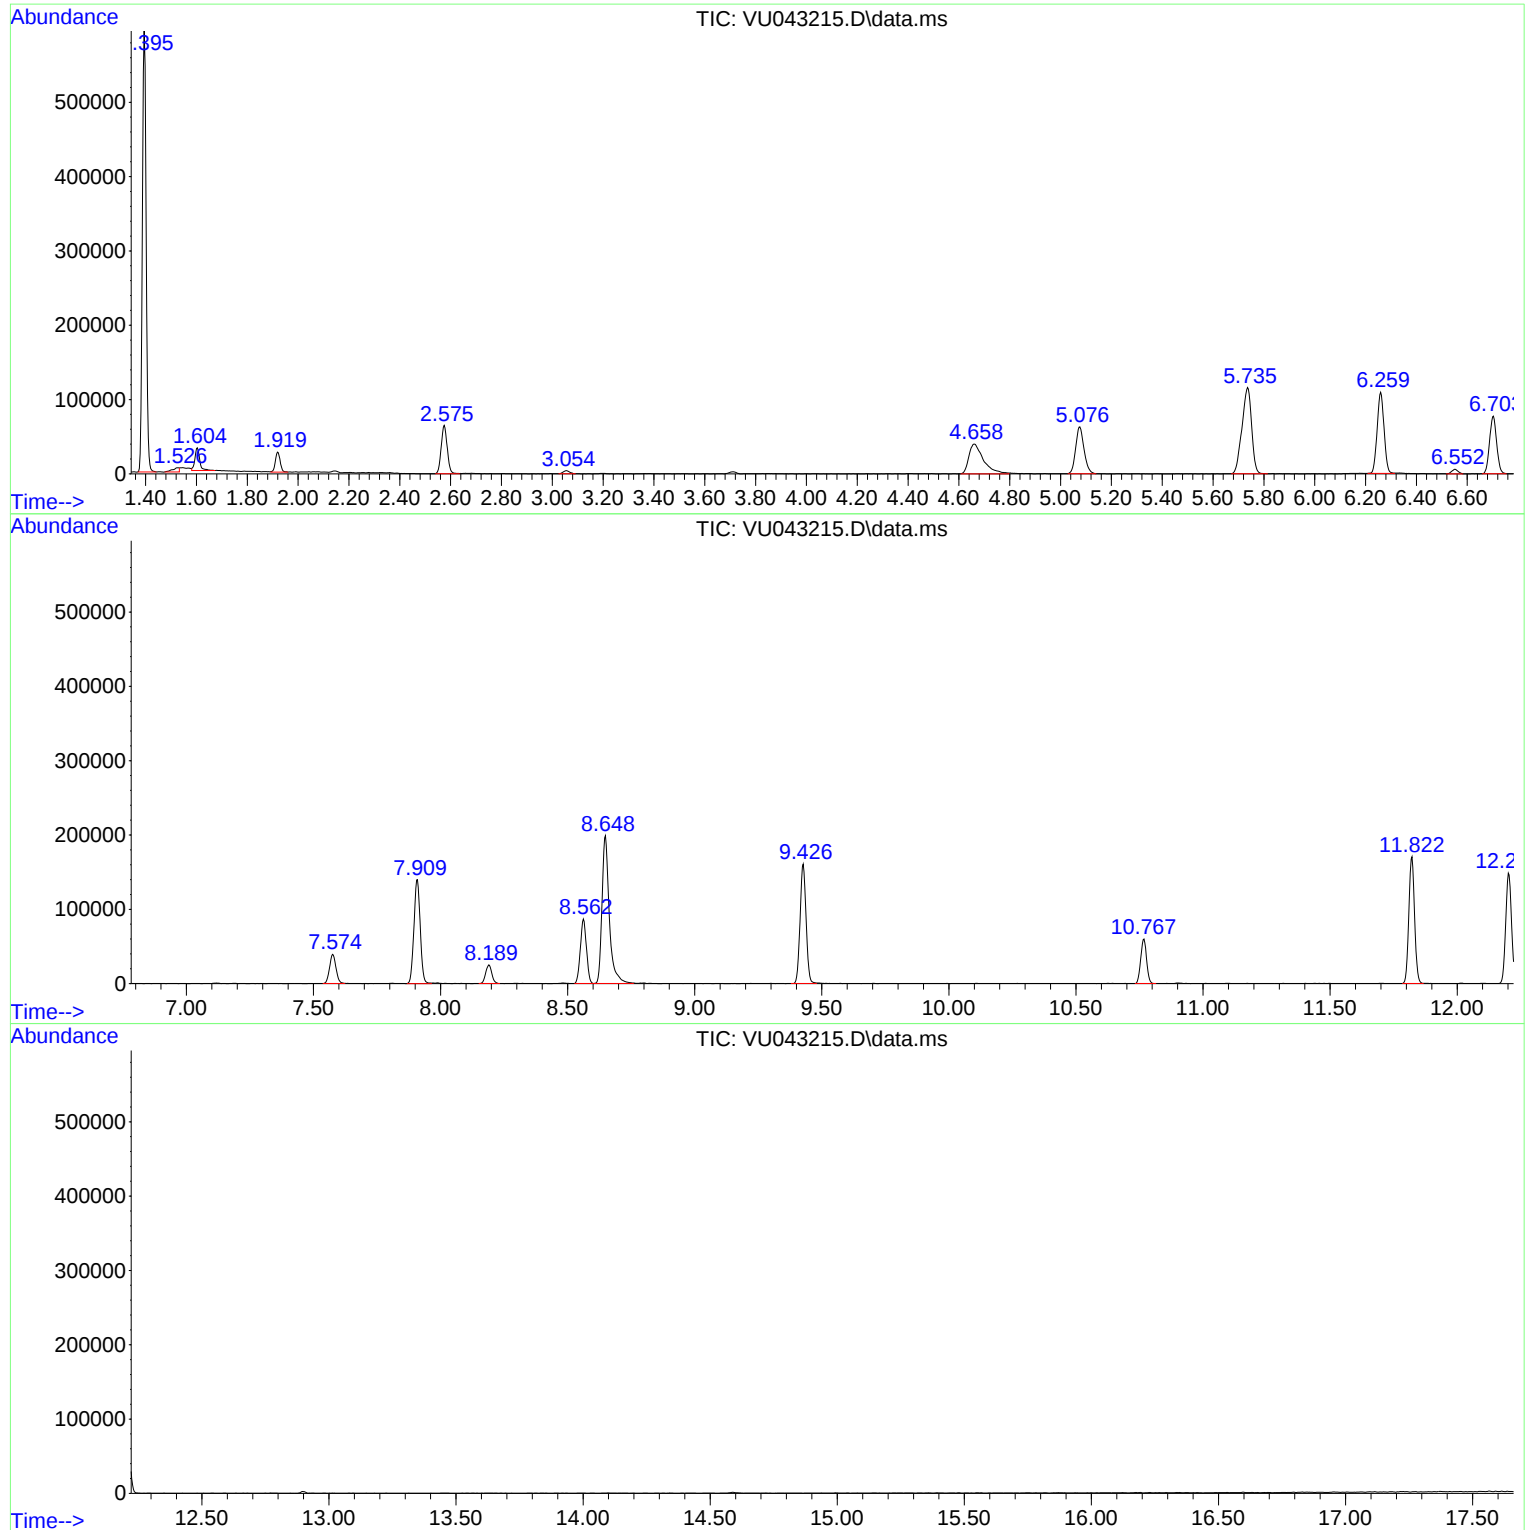

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043215.D
Acq On : 20 Apr 2021 11:52
Operator : SY/MD
Sample : M2057-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4516

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043215.D
Acq On : 20 Apr 2021 11:52
Operator : SY/MD
Sample : M2057-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4516

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
