

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
 Data File : VU043225.D
 Acq On : 20 Apr 2021 15:52
 Operator : SY/MD
 Sample : M2057-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4520

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	9	17	29	rVB	90654	90905	23.29%	2.970%
2	1.604	51	82	89	rBV	48048	121683	31.18%	3.976%
3	1.919	174	180	193	rVB	28826	39048	10.01%	1.276%
4	2.575	372	384	400	rBV	57761	96106	24.63%	3.140%
5	4.652	1013	1030	1063	rBV	48876	165277	42.35%	5.400%
6	5.076	1146	1162	1187	rVB2	60457	137087	35.13%	4.479%
7	5.736	1347	1367	1387	rBV2	111745	295896	75.83%	9.668%
8	6.256	1516	1529	1545	rBV2	111908	206933	53.03%	6.761%
9	6.549	1610	1620	1635	rVB2	17992	32540	8.34%	1.063%
10	6.700	1653	1667	1686	rBV	73729	142145	36.43%	4.644%
11	7.575	1927	1939	1956	rBV	36833	65405	16.76%	2.137%
12	7.906	2030	2042	2057	rBV	133892	225643	57.82%	7.372%
13	8.186	2119	2129	2144	rBV2	23788	39270	10.06%	1.283%
14	8.562	2234	2246	2259	rBV	88784	147203	37.72%	4.809%
15	8.645	2259	2272	2302	rBV	201443	390235	100.00%	12.750%
16	9.423	2502	2514	2533	rBV	163165	270272	69.26%	8.830%
17	10.764	2918	2931	2946	rVB	59356	93702	24.01%	3.061%
18	11.819	3247	3259	3273	rBV	168618	262060	67.15%	8.562%
19	12.070	3328	3337	3350	rBV2	9436	15387	3.94%	0.503%
20	12.201	3366	3378	3392	rVB	140779	223922	57.38%	7.316%




Sum of corrected areas: 3060719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043225.D
Acq On : 20 Apr 2021 15:52
Operator : SY/MD
Sample : M2057-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4520

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

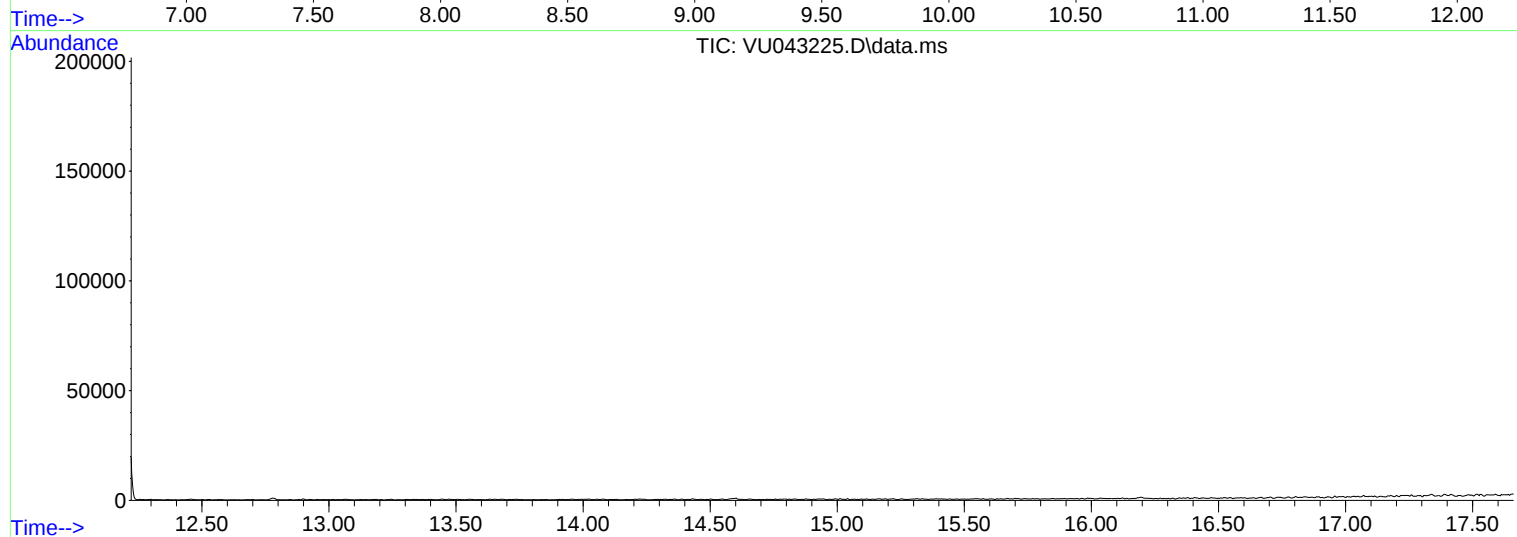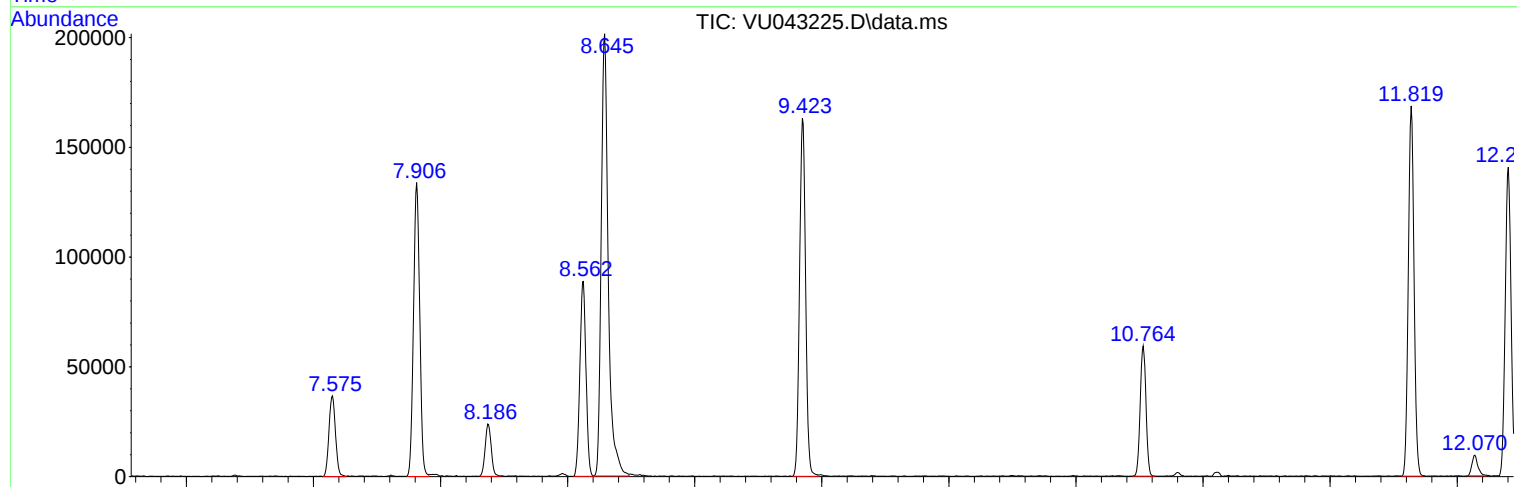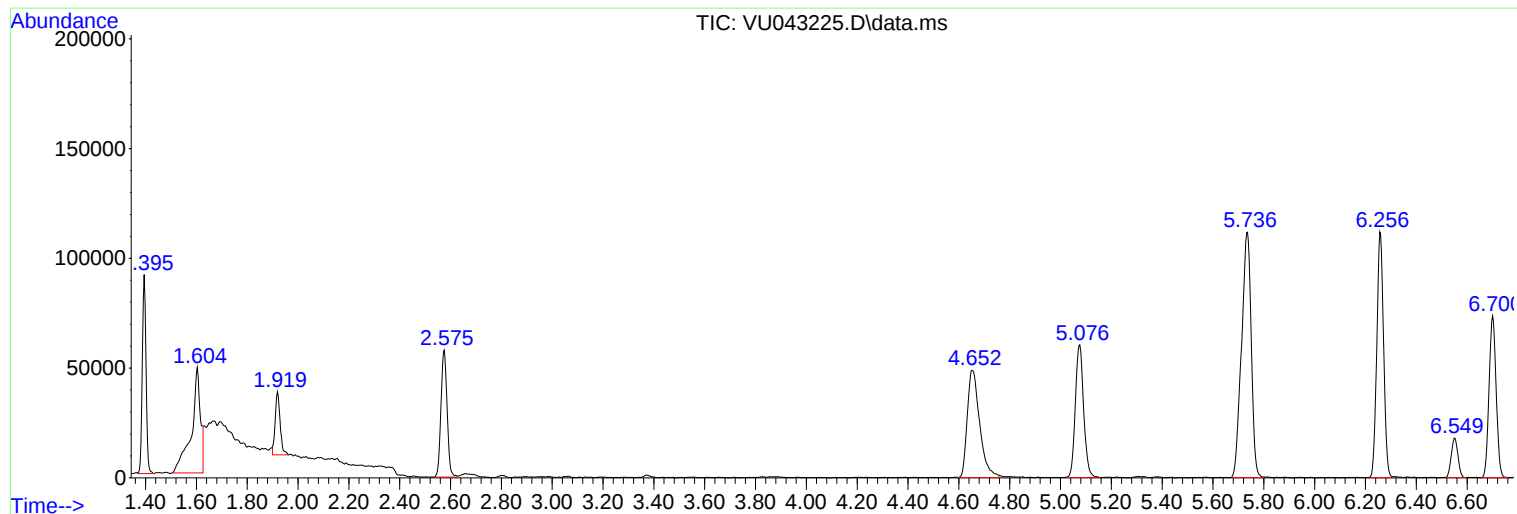

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043225.D
Acq On : 20 Apr 2021 15:52
Operator : SY/MD
Sample : M2057-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4520

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043225.D
Acq On : 20 Apr 2021 15:52
Operator : SY/MD
Sample : M2057-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4520

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
