

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
 Data File : VU043226.D
 Acq On : 20 Apr 2021 16:16
 Operator : SY/MD
 Sample : M2057-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4521

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	9	17	26	rBV	85681	89431	22.80%	2.984%
2	1.562	50	69	70	rBV6	13712	32141	8.19%	1.072%
3	1.604	75	82	88	rVV	29346	39760	10.14%	1.327%
4	1.919	173	180	190	rVB	28022	37496	9.56%	1.251%
5	2.575	372	384	396	rBV2	58944	97574	24.87%	3.256%
6	4.649	1013	1029	1058	rBV	50645	164971	42.06%	5.505%
7	5.073	1146	1161	1186	rVB2	59275	133927	34.14%	4.469%
8	5.735	1343	1367	1390	rBV2	110622	293864	74.91%	9.805%
9	6.256	1516	1529	1545	rBV	111366	205517	52.39%	6.858%
10	6.549	1610	1620	1632	rBV2	17714	32474	8.28%	1.084%
11	6.700	1653	1667	1684	rVB	75060	142206	36.25%	4.745%
12	7.571	1927	1938	1955	rBV2	35564	62010	15.81%	2.069%
13	7.906	2029	2042	2058	rBV	131279	221437	56.45%	7.389%
14	8.185	2118	2129	2145	rBV2	23828	38790	9.89%	1.294%
15	8.558	2234	2245	2259	rBV2	84053	140870	35.91%	4.700%
16	8.642	2259	2271	2299	rBV	203513	392272	100.00%	13.089%
17	9.423	2502	2514	2531	rBV	164534	271773	69.28%	9.068%
18	10.764	2920	2931	2945	rVB	57484	91720	23.38%	3.060%
19	10.899	2962	2973	2983	rBV4	2779	4213	1.07%	0.141%
20	11.819	3247	3259	3275	rBV	164991	259219	66.08%	8.649%
21	12.066	3327	3336	3353	rBV3	12154	20522	5.23%	0.685%
22	12.201	3366	3378	3394	rVB	136908	224746	57.29%	7.499%




Sum of corrected areas: 2996933

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043226.D
Acq On : 20 Apr 2021 16:16
Operator : SY/MD
Sample : M2057-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4521

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

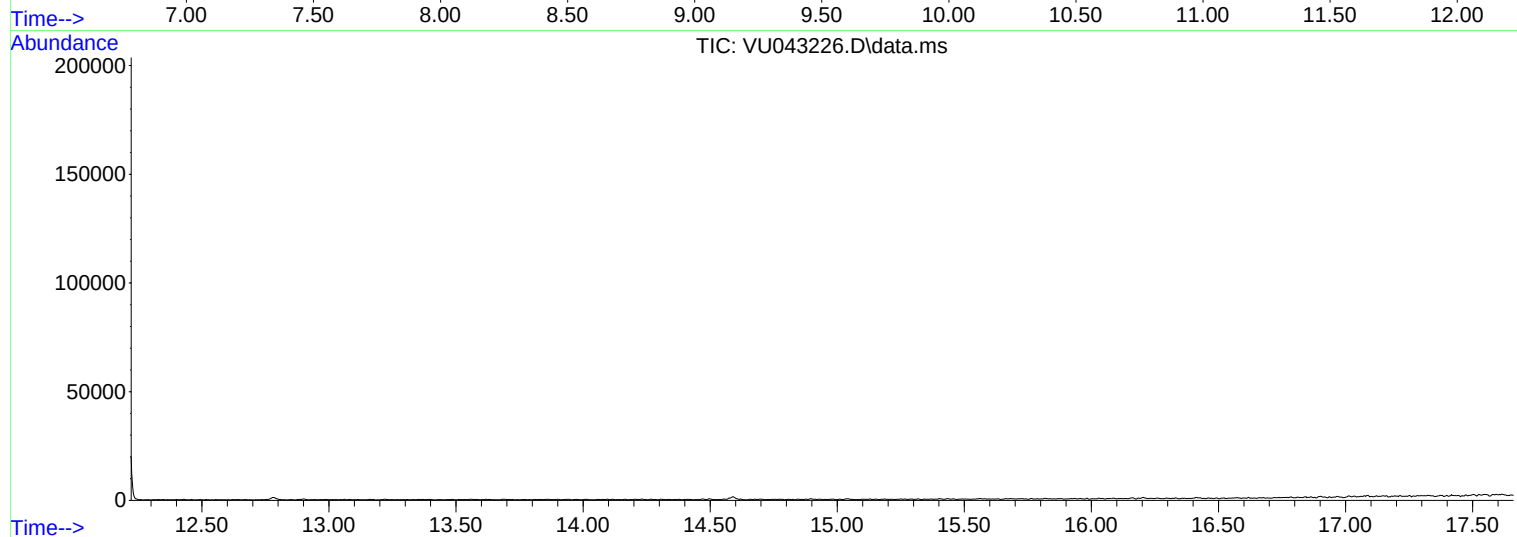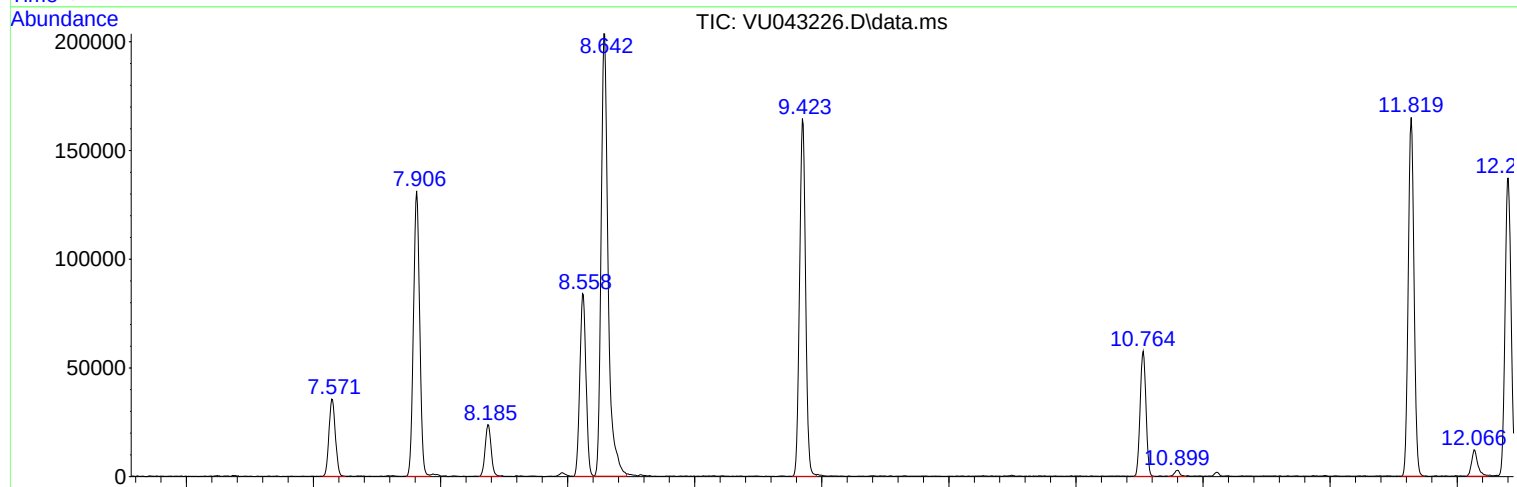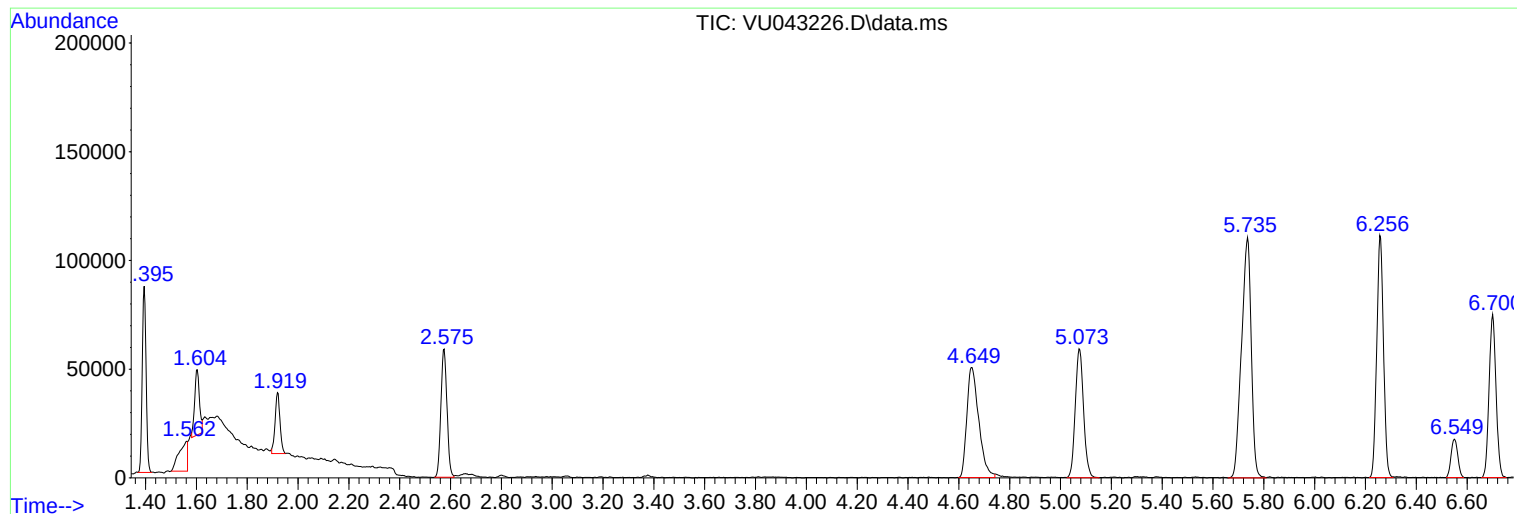

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043226.D
Acq On : 20 Apr 2021 16:16
Operator : SY/MD
Sample : M2057-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4521

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
Data File : VU043226.D
Acq On : 20 Apr 2021 16:16
Operator : SY/MD
Sample : M2057-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4521

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
