
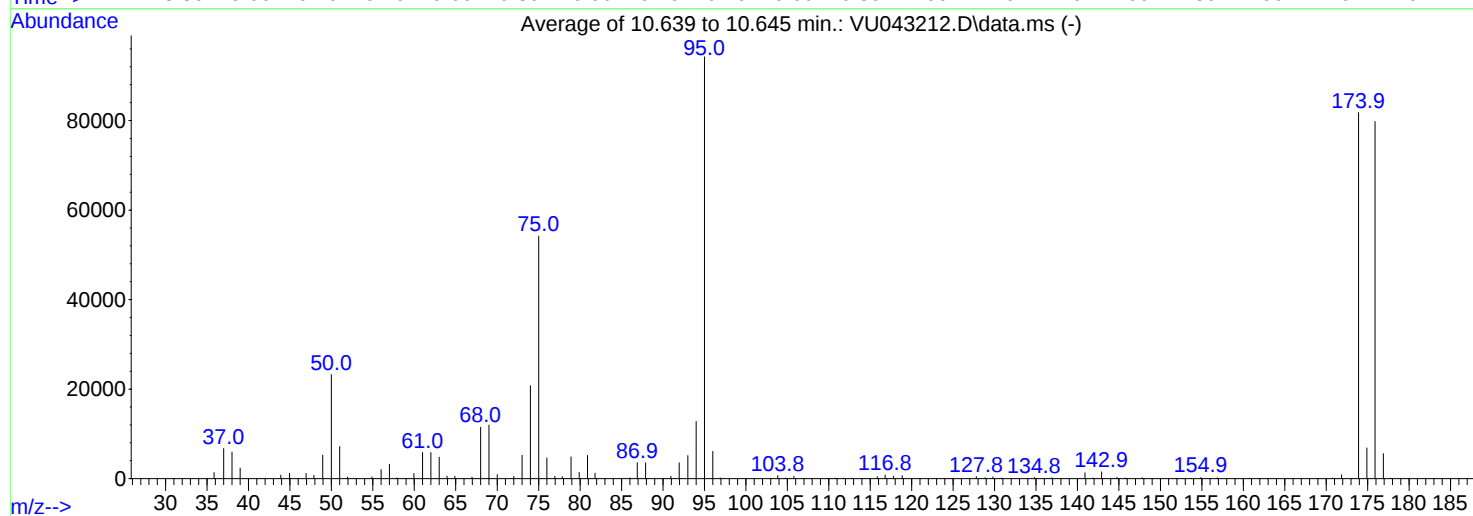


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042021\
 Data File : VU043212.D
 Acq On : 20 Apr 2021 09:08
 Operator : SY/MD
 Sample : BFB32
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB132

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Apr 22 04:40:57 2021

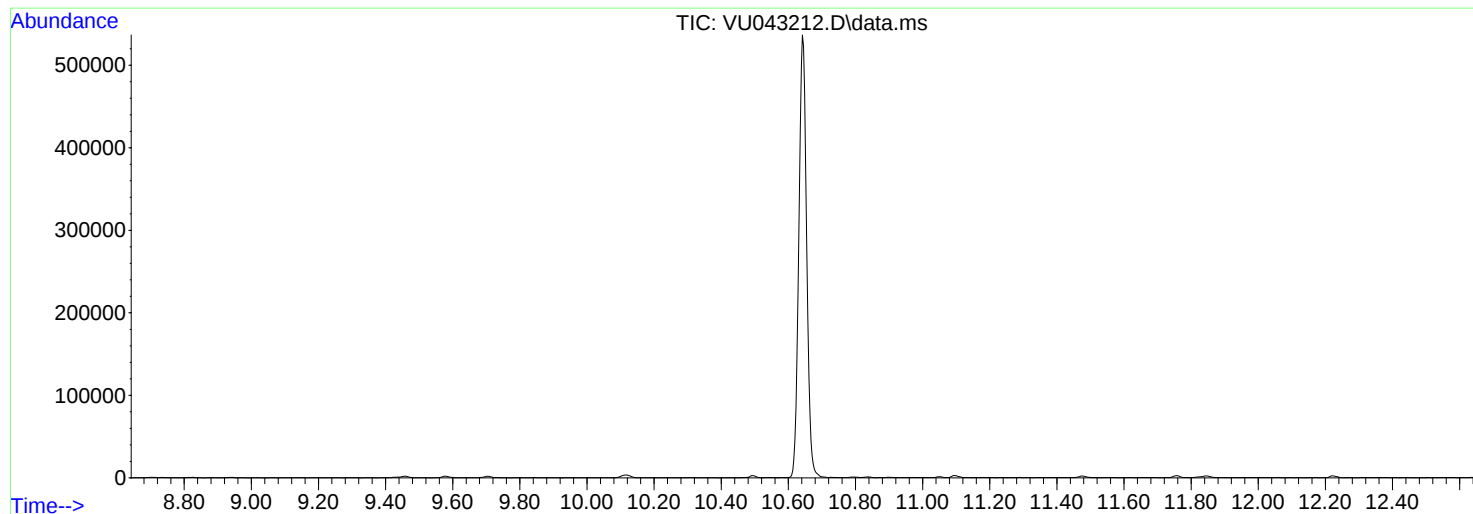

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	23240	PASS
75	95	30	80	57.5	54187	PASS
95	95	100	100	100.0	94232	PASS
96	95	5	9	6.4	6073	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	81797	PASS
175	174	5	9	8.4	6856	PASS
176	174	95	101	97.5	79781	PASS
177	176	5	9	7.0	5577	PASS

m/z	Abundance
35.90	1479.0
37.00	6444.0
38.00	5876.0
39.00	2214.0
43.90	901.0
44.90	1259.0
47.00	1134.0
47.90	736.0
48.90	5210.0
50.00	23264.0
51.00	6779.0
52.00	317.0
54.90	417.0
56.00	2032.0
57.00	3354.0
57.90	149.0
59.90	1056.0
61.00	5710.0
62.00	5806.0
63.00	4874.0
64.00	490.0
64.90	585.0
66.90	420.0
68.00	11417.0
69.00	11878.0
70.00	908.0
72.00	612.0
73.00	5106.0
74.00	20552.0
75.00	54160.0
76.00	4733.0
76.90	542.0
77.80	487.0
78.90	4873.0
79.90	1427.0
80.90	5185.0
81.80	1236.0
83.00	112.0
86.00	133.0
86.90	3542.0
87.90	3501.0
90.90	485.0
92.00	3619.0
93.00	5307.0
94.00	12684.0
95.00	94944.0
96.00	5974.0
96.90	151.0
103.90	640.0
104.80	154.0
105.80	523.0
110.80	174.0
111.80	117.0
112.90	130.0
115.80	503.0
116.80	866.0
117.80	517.0
118.90	683.0
127.80	434.0
128.80	226.0
129.80	392.0
130.80	148.0
134.80	217.0
137.00	137.0
140.90	1423.0
141.80	111.0
142.90	1575.0
144.80	268.0
145.70	128.0
147.80	242.0
154.90	322.0
156.90	184.0
160.70	108.0
170.80	138.0
171.80	813.0
173.90	83304.0
174.90	7217.0
175.90	81728.0
176.90	5584.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.90	1356.0
37.00	6769.0
38.00	5792.0
39.00	2408.0
40.10	100.0
43.90	1044.0
45.00	1187.0
45.90	155.0
46.90	1166.0
47.90	749.0
49.00	5171.0
50.00	22424.0
51.00	7327.0
51.90	358.0
53.00	129.0
54.90	341.0
56.00	1965.0
57.00	3044.0
57.90	203.0
60.00	1189.0
61.00	5735.0
62.00	5717.0
63.00	4507.0
63.90	621.0
64.90	523.0
67.00	296.0
68.00	11226.0
69.00	11606.0
70.00	827.0
72.00	462.0
73.00	5127.0
74.00	20376.0
75.00	52744.0
76.00	4419.0
77.00	512.0
77.90	440.0
78.90	4734.0
79.90	1328.0
80.90	5008.0
81.80	1201.0
86.00	241.0
86.90	3530.0
87.90	3519.0
91.00	500.0
91.90	3371.0
93.00	4852.0
94.00	12511.0
95.00	90528.0
96.00	6012.0
96.90	164.0
103.80	679.0
104.70	117.0
105.80	546.0
109.90	110.0
111.80	110.0
112.70	109.0
114.90	101.0
115.80	442.0
116.80	742.0
117.80	537.0
118.80	663.0
127.80	442.0
128.90	191.0
129.80	385.0
130.90	126.0
134.80	244.0
136.80	207.0
140.90	1165.0
141.90	147.0
142.90	1388.0
144.80	286.0
145.80	157.0
147.80	196.0
153.80	123.0
154.90	262.0
156.80	183.0
160.80	100.0
170.80	139.0
171.90	894.0
173.90	77792.0
174.90	6267.0
175.90	75264.0
176.90	5305.0
177.80	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.90	105.0
39.90	125.0
43.90	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.90	1530.0
37.00	6925.0
38.00	6140.0
39.00	2463.0
43.90	1027.0
44.90	1255.0
45.90	114.0
46.90	1219.0
47.90	820.0
49.00	5424.0
50.00	24032.0
51.00	7451.0
51.90	356.0
54.90	407.0
56.00	2103.0
57.00	3300.0
57.90	196.0
59.90	1150.0
61.00	6023.0
62.00	6018.0
63.00	5002.0
63.90	565.0
64.90	554.0
66.90	356.0
68.00	11791.0
69.00	12401.0
70.00	904.0
72.00	574.0
73.00	5448.0
74.00	21392.0
75.00	55656.0
76.00	4838.0
77.00	528.0
77.90	470.0
78.90	5029.0
79.90	1434.0
80.90	5387.0
81.80	1269.0
86.00	223.0
86.90	3678.0
87.90	3642.0
91.00	494.0
91.90	3654.0
93.00	5240.0
94.00	13220.0
95.00	97224.0
96.00	6232.0
96.90	180.0
103.90	718.0
104.80	141.0
105.80	579.0
109.80	114.0
110.80	151.0
111.80	128.0
112.80	122.0
115.90	488.0
116.80	842.0
117.80	527.0
118.80	680.0
127.80	469.0
128.80	205.0
129.80	416.0
130.90	132.0
134.80	250.0
136.90	164.0
140.90	1368.0
142.00	138.0
142.90	1532.0
144.70	280.0
145.70	126.0
147.80	223.0
153.70	136.0
154.90	308.0
156.90	186.0
160.80	105.0
170.80	153.0
171.80	892.0
173.90	84296.0
174.90	7085.0
175.90	82352.0
176.90	5841.0
177.80	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132