




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048153.D
 Acq On : 20 Apr 2022 19:13
 Operator : SY/MD
 Sample : N2485-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J18

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/21/2022
 Supervised By :Mahesh Dadoda 04/21/2022

Quant Time: Apr 21 02:44:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 21 02:37:57 2022
 Response via : Initial Calibration

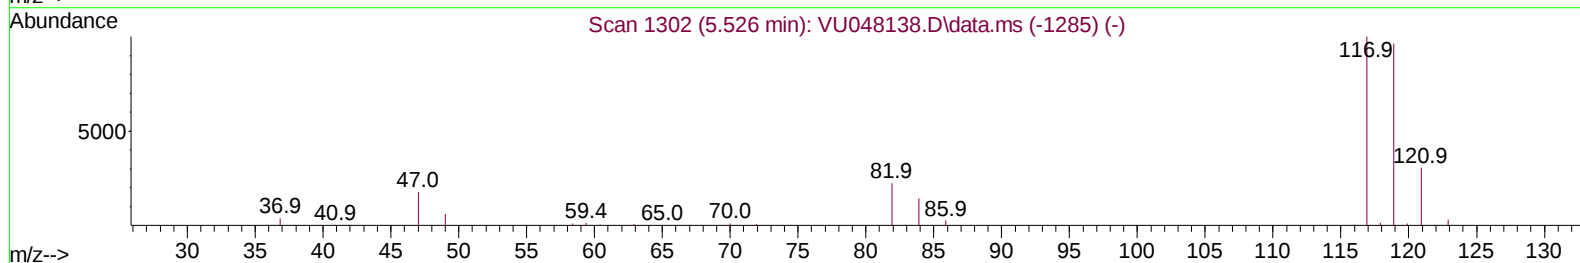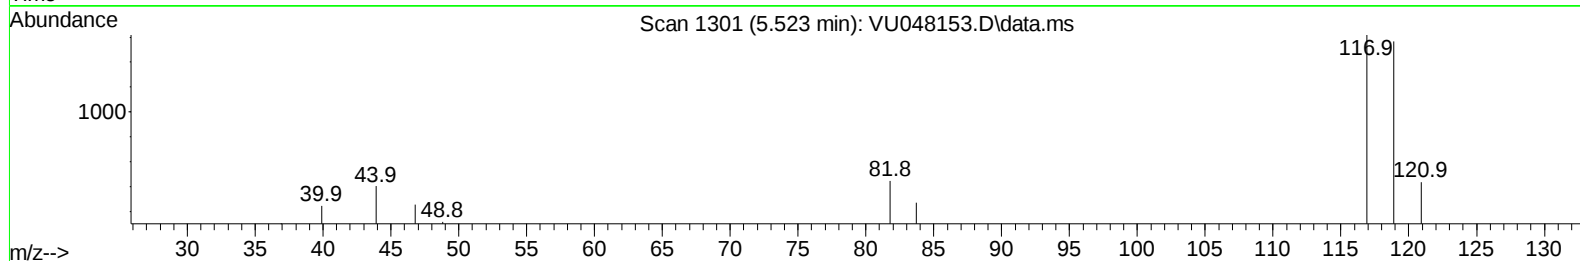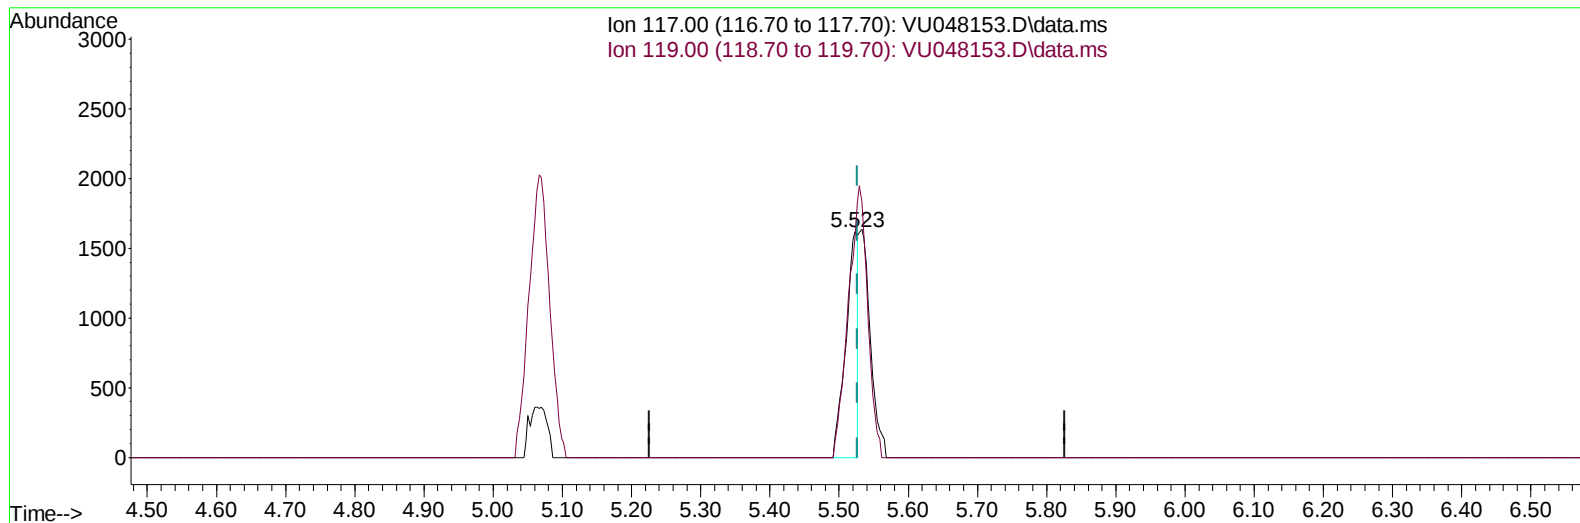

TIC: VU048153.D\data.ms

(31) Carbon tetrachloride (T)

5.523min (-0.003) 0.53 ug/L

response 1941

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	96.50	193.71#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048153.D
Acq On : 20 Apr 2022 19:13
Operator : SY/MD
Sample : N2485-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J18

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/21/2022
Supervised By :Mahesh Dadoda 04/21/2022

Quant Time: Apr 21 02:44:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 21 02:37:57 2022
Response via : Initial Calibration

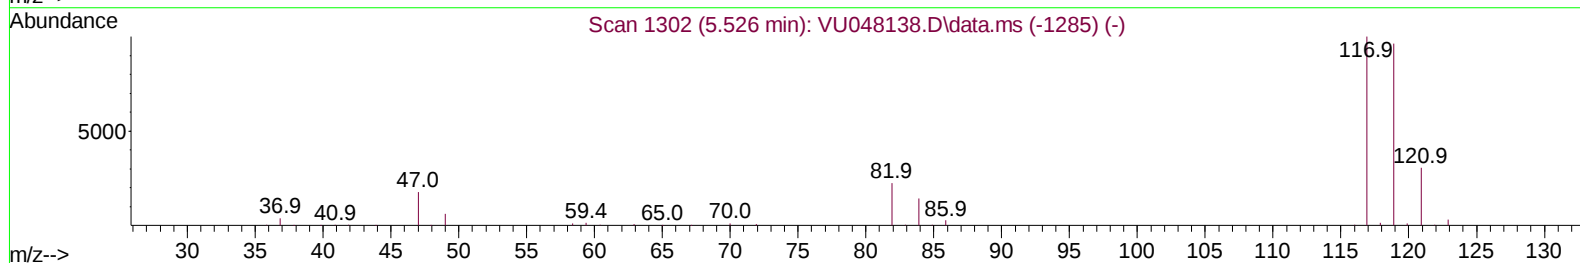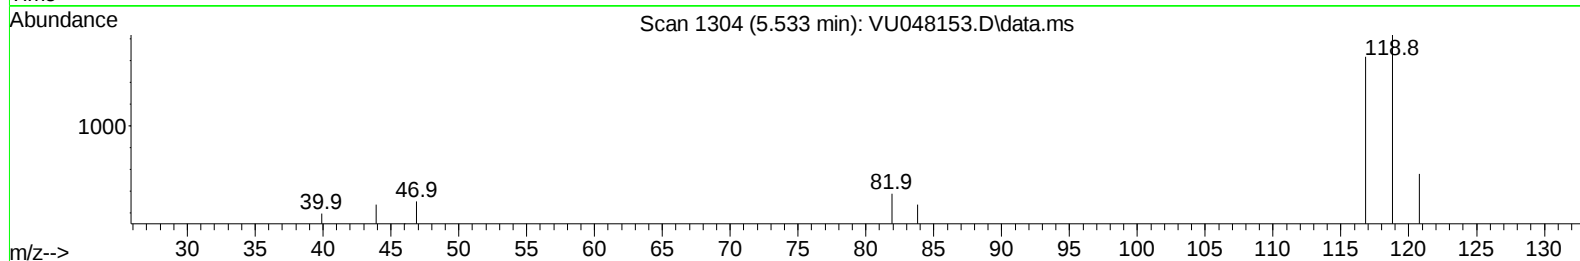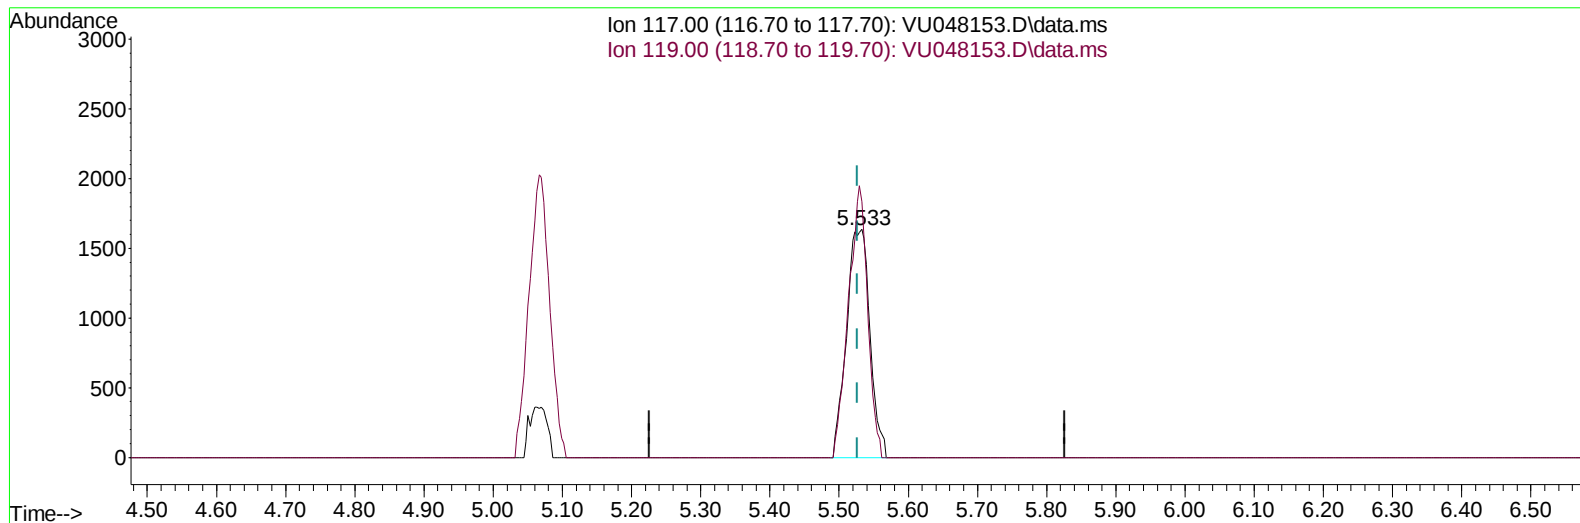

TIC: VU048153.D\data.ms

(31) Carbon tetrachloride (T)

5.533min (+ 0.006) 1.04 ug/L m

response 3834

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	96.50	98.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048153.D
 Acq On : 20 Apr 2022 19:13
 Operator : SY/MD
 Sample : N2485-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J18

Manual IntegrationsAPPROVED

Quant Time: Apr 21 02:44:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 21 02:37:57 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 04/21/2022
 Supervised By : Mahesh Dadoda 04/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	350267	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	359629	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	190164	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	108746	42.813	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	85.620%	
7) Chloroethane-d5	1.916	69	90656	45.265	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	90.520%	
11) 1,1-Dichloroethene-d2	2.571	63	143678	30.917	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	61.840%	
21) 2-Butanone-d5	4.626	46	183600	84.214	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	84.210%	
24) Chloroform-d	5.067	84	205234	44.160	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.320%	
26) 1,2-Dichloroethane-d4	5.703	65	128448	45.063	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.120%	
32) Benzene-d6	5.729	84	416750	46.053	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	92.100%	
36) 1,2-Dichloropropane-d6	6.694	67	135693	48.826	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	97.660%	
41) Toluene-d8	7.899	98	363384	41.216	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	82.440%	
43) trans-1,3-Dichloroprop...	8.179	79	56741	40.300	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	80.600%	
47) 2-Hexanone-d5	8.632	63	131762	80.990	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	80.990%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	208638	43.745	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.480%	
66) 1,2-Dichlorobenzene-d4	12.192	152	168239	49.728	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.460%	
Target Compounds						
					Qvalue	
31) Carbon tetrachloride	5.533	117	3834m	1.041	ug/L	
33) Benzene	5.777	78	2753410	264.508	ug/L	100
51) Chlorobenzene	9.449	112	3807865	491.004	ug/L	98
64) 1,3-Dichlorobenzene	11.745	146	107517	18.822	ug/L	99
65) 1,4-Dichlorobenzene	11.835	146	1447977	244.720	ug/L	100
67) 1,2-Dichlorobenzene	12.214	146	1175333	205.629	ug/L	99
70) 1,2,4-trichlorobenzene	13.841	180	122978	30.263	ug/L	99
72) 1,2,3-Trichlorobenzene	14.330	180	24792	6.086	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048153.D
Acq On : 20 Apr 2022 19:13
Operator : SY/MD
Sample : N2485-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J18

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/21/2022
Supervised By :Mahesh Dadoda 04/21/2022

Quant Time: Apr 21 02:44:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 21 02:37:57 2022
Response via : Initial Calibration

