

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048142.D
 Acq On : 20 Apr 2022 15:00
 Operator : SY/MD
 Sample : N2485-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J00

Quant Time: Apr 21 02:42:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 21 02:37:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	334862	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	343167	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	177554	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	112085	46.158	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.320%
7) Chloroethane-d5	1.915	69	92952	48.546	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.100%
11) 1,1-Dichloroethene-d2	2.568	63	145107	32.661	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.320%
21) 2-Butanone-d5	4.626	46	184181	88.367	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.370%
24) Chloroform-d	5.066	84	203439	45.787	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.580%
26) 1,2-Dichloroethane-d4	5.703	65	127481	46.781	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.560%
32) Benzene-d6	5.729	84	407464	47.187	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.380%
36) 1,2-Dichloropropane-d6	6.693	67	135387	51.053	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.100%
41) Toluene-d8	7.899	98	351849	41.822	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.640%
43) trans-1,3-Dichloroprop...	8.179	79	55842	41.564	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.120%
47) 2-Hexanone-d5	8.635	63	116739	75.198	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.200%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	205729	45.204	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	154432	48.889	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.780%
Target Compounds					Qvalue	
13) Acetone	2.636	43	9024	4.652	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048142.D
Acq On : 20 Apr 2022 15:00
Operator : SY/MD
Sample : N2485-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J00

Quant Time: Apr 21 02:42:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 21 02:37:57 2022
Response via : Initial Calibration

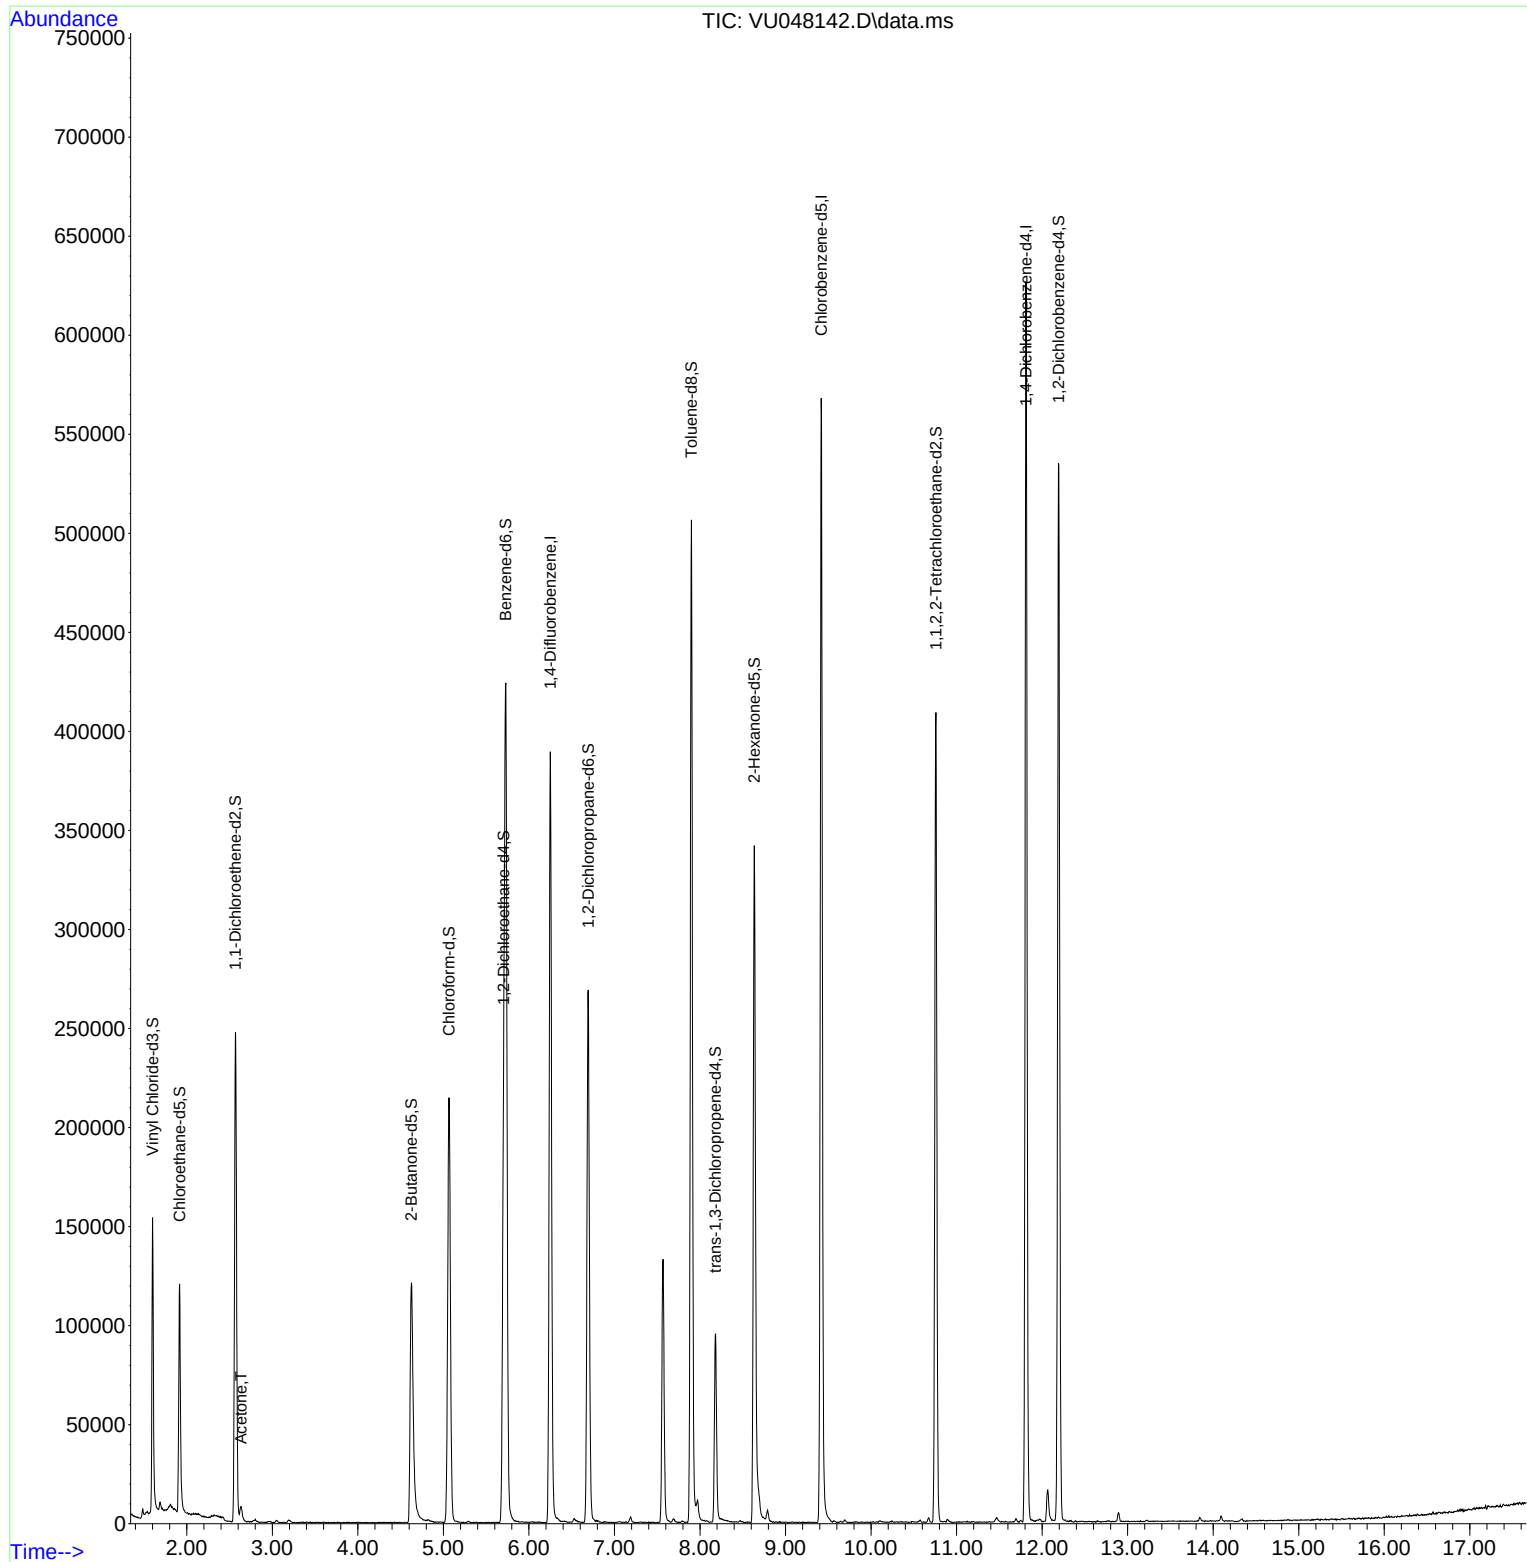

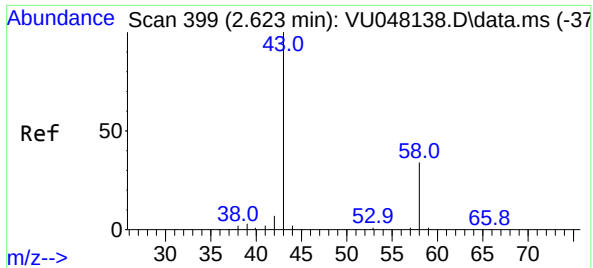

#13
 Acetone
 Concen: 4.652 ug/L
 RT: 2.636 min Scan# 40
 Delta R.T. 0.013 min
 Lab File: VU048142.D
 Acq: 20 Apr 2022 15:00

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J00

Tgt Ion: 43 Resp: 9024
 Ion Ratio Lower Upper
 43 100
 58 36.0 0.0 70.0

