

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048145.D
 Acq On : 20 Apr 2022 16:09
 Operator : SY/MD
 Sample : N2485-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX9

Quant Time: Apr 21 02:42:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 21 02:37:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	327462	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	348510	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	172869	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	111998	47.164	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.320%
7) Chloroethane-d5	1.916	69	94050	50.230	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.460%
11) 1,1-Dichloroethene-d2	2.568	63	144502	33.260	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.520%
21) 2-Butanone-d5	4.620	46	185532	91.027	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.030%
24) Chloroform-d	5.067	84	209401	48.194	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.380%
26) 1,2-Dichloroethane-d4	5.703	65	128758	48.317	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.640%
32) Benzene-d6	5.729	84	421344	48.047	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.100%
36) 1,2-Dichloropropane-d6	6.690	67	137483	51.048	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.100%
41) Toluene-d8	7.899	98	360034	42.138	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.280%
43) trans-1,3-Dichloroprop...	8.179	79	57232	41.946	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.900%
47) 2-Hexanone-d5	8.632	63	125280	79.462	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.460%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	210315	45.503	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.000%
66) 1,2-Dichlorobenzene-d4	12.192	152	156493	50.884	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.760%
Target Compounds						
13) Acetone	2.626	43	9670	5.098	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048145.D
Acq On : 20 Apr 2022 16:09
Operator : SY/MD
Sample : N2485-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX9


Quant Time: Apr 21 02:42:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 21 02:37:57 2022
Response via : Initial Calibration

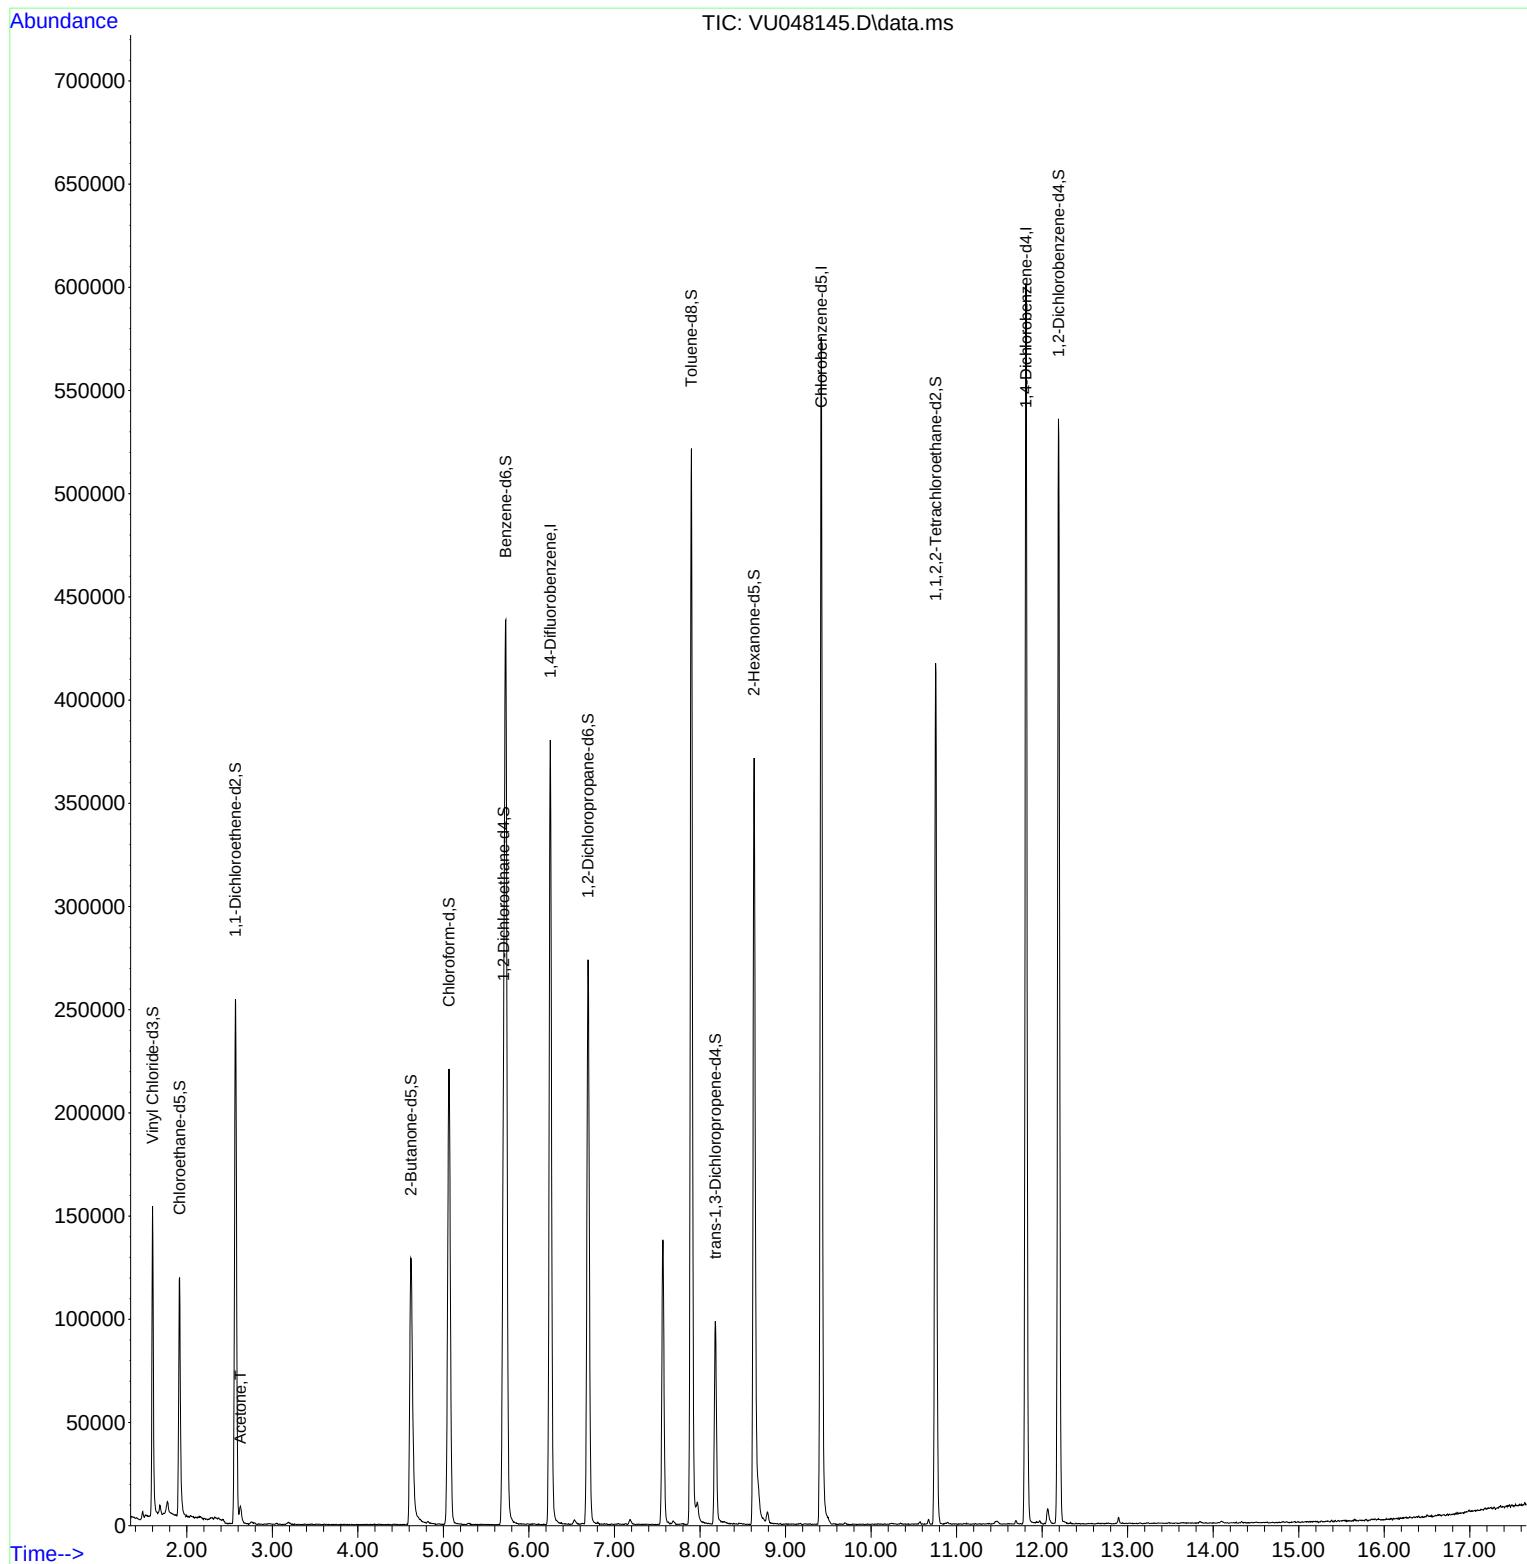

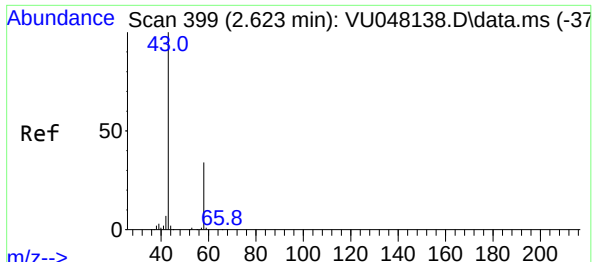

#13
 Acetone
 Concen: 5.098 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU048145.D
 Acq: 20 Apr 2022 16:09

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX9

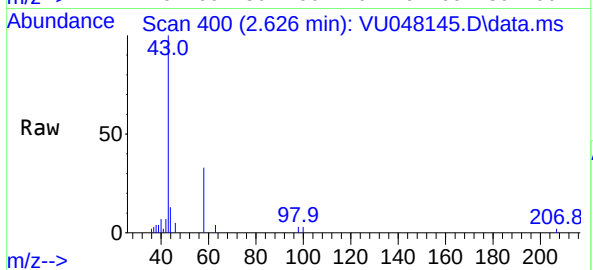

Tgt Ion: 43 Resp: 9670
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 70.0

