

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048139.D
 Acq On : 20 Apr 2022 13:51
 Operator : SY/MD
 Sample : VU0420WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048139.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	106	rBV	152971	185958	15.17%	1.872%
2	1.916	171	179	202	rVB	125051	179671	14.65%	1.808%
3	2.285	292	294	299	rVB3	1001	668	0.05%	0.007%
4	2.568	369	382	404	rBV	249747	423673	34.55%	4.264%
5	2.720	424	429	430	rBV3	444	317	0.03%	0.003%
6	2.797	446	453	457	rBV2	925	1306	0.11%	0.013%
7	2.964	498	505	510	rBV3	443	635	0.05%	0.006%
8	3.054	524	533	542	rVB5	2065	4291	0.35%	0.043%
9	3.192	565	576	586	rBV3	1202	2548	0.21%	0.026%
10	3.356	623	627	631	rVV4	544	502	0.04%	0.005%
11	3.543	681	685	690	rVV2	243	281	0.02%	0.003%
12	3.642	710	716	720	rBV2	175	207	0.02%	0.002%
13	3.774	752	757	761	rBV2	226	227	0.02%	0.002%
14	3.932	802	806	809	rBV2	256	219	0.02%	0.002%
15	4.012	827	831	837	rBV2	199	252	0.02%	0.003%
16	4.170	876	880	884	rBV2	177	178	0.01%	0.002%
17	4.195	884	888	893	rVB2	187	186	0.02%	0.002%
18	4.237	893	901	904	rBV2	294	343	0.03%	0.003%
19	4.633	1006	1024	1061	rBV	126025	344872	28.12%	3.471%
20	5.067	1142	1159	1181	rVV	223378	490003	39.96%	4.931%
21	5.192	1195	1198	1201	rVB2	338	213	0.02%	0.002%
22	5.253	1212	1217	1219	rBV3	326	263	0.02%	0.003%
23	5.289	1224	1228	1237	rBV3	629	830	0.07%	0.008%
24	5.324	1237	1239	1243	rVV2	336	180	0.01%	0.002%
25	5.527	1299	1302	1307	rVV3	272	246	0.02%	0.002%
26	5.729	1343	1365	1395	rBV2	450002	1226217	100.00%	12.341%
27	6.041	1457	1462	1469	rVB2	557	865	0.07%	0.009%
28	6.086	1469	1476	1481	rBV3	369	554	0.05%	0.006%
29	6.170	1499	1502	1506	rVB3	274	224	0.02%	0.002%
30	6.253	1513	1528	1554	rBV	385283	741695	60.49%	7.465%
31	6.465	1592	1594	1602	rVB3	420	354	0.03%	0.004%
32	6.536	1604	1616	1628	rVB9	2298	5095	0.42%	0.051%
33	6.588	1628	1632	1633	rBV2	367	209	0.02%	0.002%
34	6.694	1649	1665	1685	rBV	285440	554170	45.19%	5.577%
35	6.800	1693	1698	1708	rVB6	877	1518	0.12%	0.015%
36	6.970	1747	1751	1756	rBV2	198	215	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048139.D
 Acq On : 20 Apr 2022 13:51
 Operator : SY/MD
 Sample : VU0420WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.041	1770	1773	1775	rBV	437	269	0.02%	0.003%
38	7.189	1811	1819	1830	rBV4	2741	4908	0.40%	0.049%
39	7.301	1849	1854	1857	rBV2	261	229	0.02%	0.002%
40	7.568	1924	1937	1964	rBV	144580	258336	21.07%	2.600%
41	7.687	1968	1974	1975	rBV3	989	904	0.07%	0.009%
42	7.735	1986	1989	1993	rVB2	273	215	0.02%	0.002%
43	7.797	2001	2008	2019	rVB6	2554	4104	0.33%	0.041%
44	7.899	2027	2040	2055	rBV	541965	945144	77.08%	9.512%
45	8.182	2115	2128	2150	rBV	102504	179342	14.63%	1.805%
46	8.356	2179	2182	2185	rBV2	321	223	0.02%	0.002%
47	8.427	2202	2204	2207	rVB	374	176	0.01%	0.002%
48	8.523	2231	2234	2236	rBV2	327	265	0.02%	0.003%
49	8.559	2242	2245	2250	rVB4	551	345	0.03%	0.003%
50	8.639	2254	2270	2315	rBV	395335	748070	61.01%	7.529%
51	8.874	2338	2343	2346	rVV3	349	360	0.03%	0.004%
52	8.925	2356	2359	2365	rVB3	822	835	0.07%	0.008%
53	9.079	2405	2407	2412	rVB3	343	301	0.02%	0.003%
54	9.128	2417	2422	2424	rBV3	248	227	0.02%	0.002%
55	9.166	2429	2434	2436	rVV3	441	330	0.03%	0.003%
56	9.420	2496	2513	2534	rBV	549373	927358	75.63%	9.333%
57	9.578	2553	2562	2567	rBV5	776	1156	0.09%	0.012%
58	9.610	2569	2572	2575	rVB2	416	258	0.02%	0.003%
59	9.697	2590	2599	2605	rBV3	1382	1741	0.14%	0.018%
60	9.803	2629	2632	2637	rVB2	253	204	0.02%	0.002%
61	9.938	2670	2674	2678	rBV2	232	236	0.02%	0.002%
62	10.002	2688	2694	2698	rBV2	265	362	0.03%	0.004%
63	10.025	2698	2701	2707	rVV	170	187	0.02%	0.002%
64	10.108	2719	2727	2738	rBV4	1288	2373	0.19%	0.024%
65	10.227	2759	2764	2768	rBV2	150	178	0.01%	0.002%
66	10.353	2795	2803	2806	rVV	267	324	0.03%	0.003%
67	10.485	2835	2844	2853	rVB3	850	1365	0.11%	0.014%
68	10.642	2890	2893	2894	rBV2	369	210	0.02%	0.002%
69	10.674	2897	2903	2915	rVB5	2239	3549	0.29%	0.036%
70	10.758	2915	2929	2946	rBV	429539	703744	57.39%	7.083%
71	10.870	2960	2964	2968	rBV3	333	348	0.03%	0.004%
72	10.899	2970	2973	2975	rVV2	509	258	0.02%	0.003%
73	11.086	3028	3031	3039	rVB	622	864	0.07%	0.009%
74	11.121	3039	3042	3046	rBV3	561	449	0.04%	0.005%
75	11.465	3142	3149	3150	rBV4	1971	2165	0.18%	0.022%
76	11.520	3164	3166	3169	rVB	479	265	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048139.D
 Acq On : 20 Apr 2022 13:51
 Operator : SY/MD
 Sample : VU0420WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.546	3170	3174	3180	rBV2	241	285	0.02%	0.003%
78	11.584	3181	3186	3187	rBV3	437	354	0.03%	0.004%
79	11.700	3216	3222	3226	rBV4	744	849	0.07%	0.009%
80	11.751	3230	3238	3244	rVB3	1657	2613	0.21%	0.026%
81	11.812	3244	3257	3285	rBV	617145	995059	81.15%	10.014%
82	12.121	3349	3353	3357	rVB3	475	339	0.03%	0.003%
83	12.195	3362	3376	3395	rVV	567674	928239	75.70%	9.342%
84	12.308	3408	3411	3416	rVB3	622	534	0.04%	0.005%
85	12.330	3416	3418	3422	rBV3	512	307	0.03%	0.003%
86	12.362	3425	3428	3431	rBV2	506	296	0.02%	0.003%
87	12.378	3431	3433	3437	rBV2	391	176	0.01%	0.002%
88	12.414	3440	3444	3448	rBV2	215	203	0.02%	0.002%
89	12.481	3462	3465	3468	rBV3	341	266	0.02%	0.003%
90	12.613	3501	3506	3510	rBV3	424	443	0.04%	0.004%
91	12.996	3623	3625	3626	rBV	544	265	0.02%	0.003%
92	13.063	3644	3646	3651	rBV2	365	243	0.02%	0.002%
93	13.179	3678	3682	3684	rBV2	379	323	0.03%	0.003%
94	13.227	3689	3697	3708	rVB5	2627	4546	0.37%	0.046%
95	13.845	3881	3889	3898	rBV2	5175	7302	0.60%	0.073%
96	14.092	3958	3966	3981	rVB	13070	21715	1.77%	0.219%
97	14.333	4033	4041	4053	rBV4	5258	8790	0.72%	0.088%
98	14.835	4193	4197	4200	rBV2	432	460	0.04%	0.005%
99	15.131	4286	4289	4291	rBV3	596	449	0.04%	0.005%
100	15.507	4403	4406	4410	rBV3	917	786	0.06%	0.008%




Sum of corrected areas: 9936204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048139.D
Acq On : 20 Apr 2022 13:51
Operator : SY/MD
Sample : VU0420WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

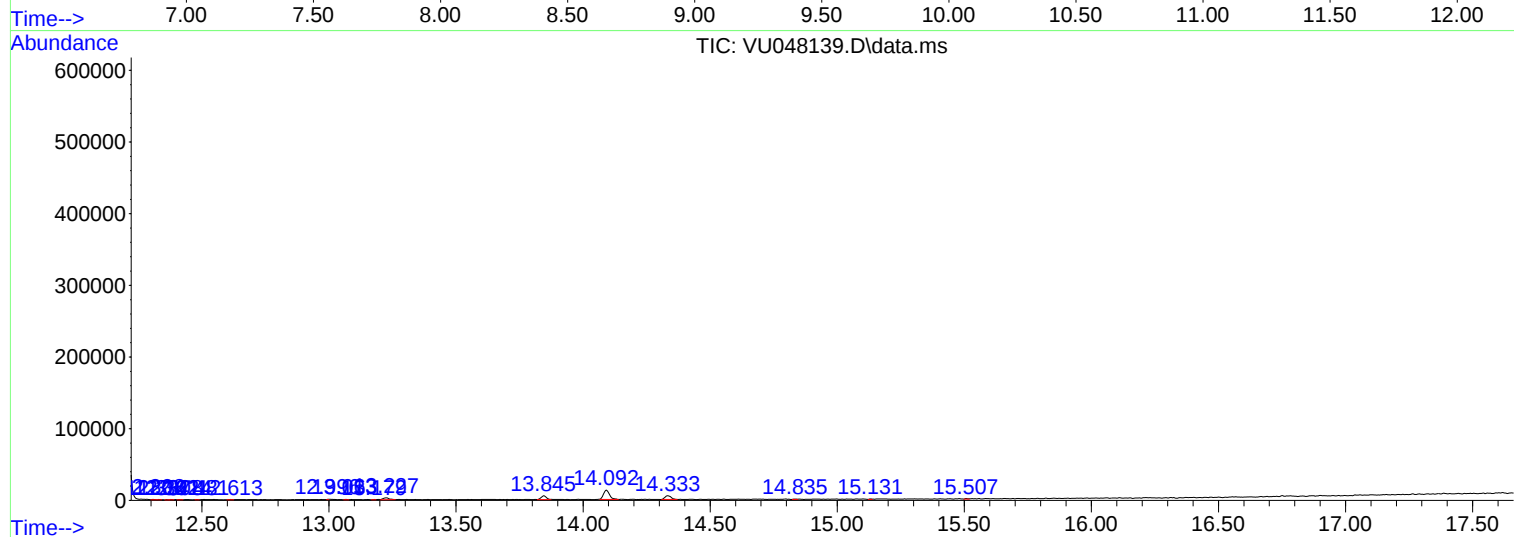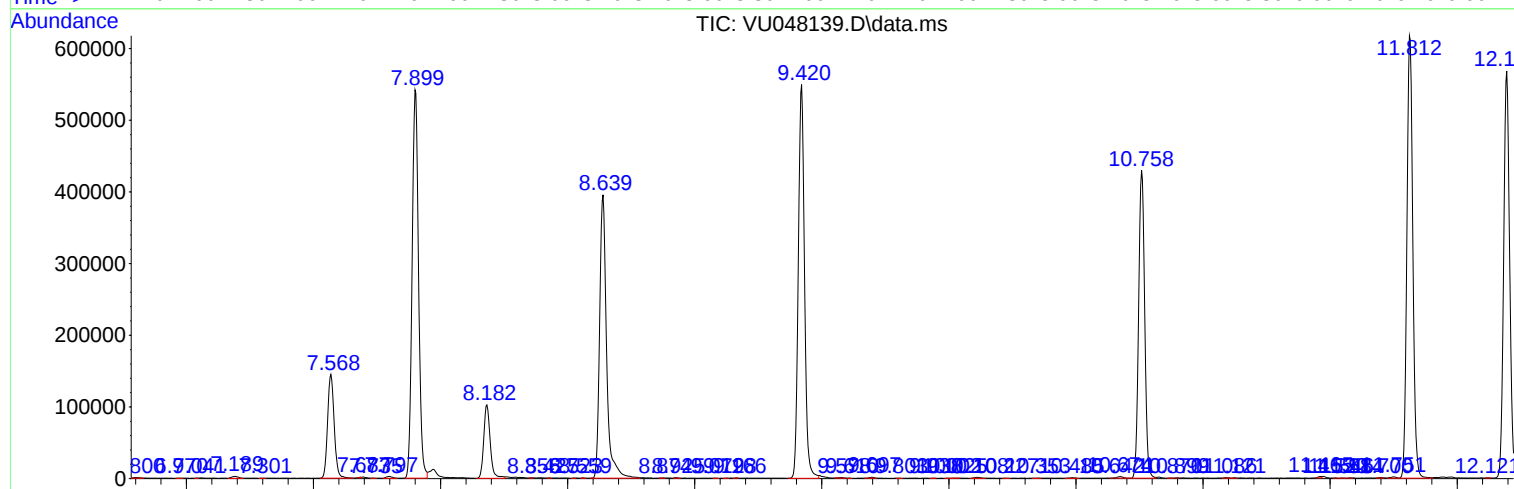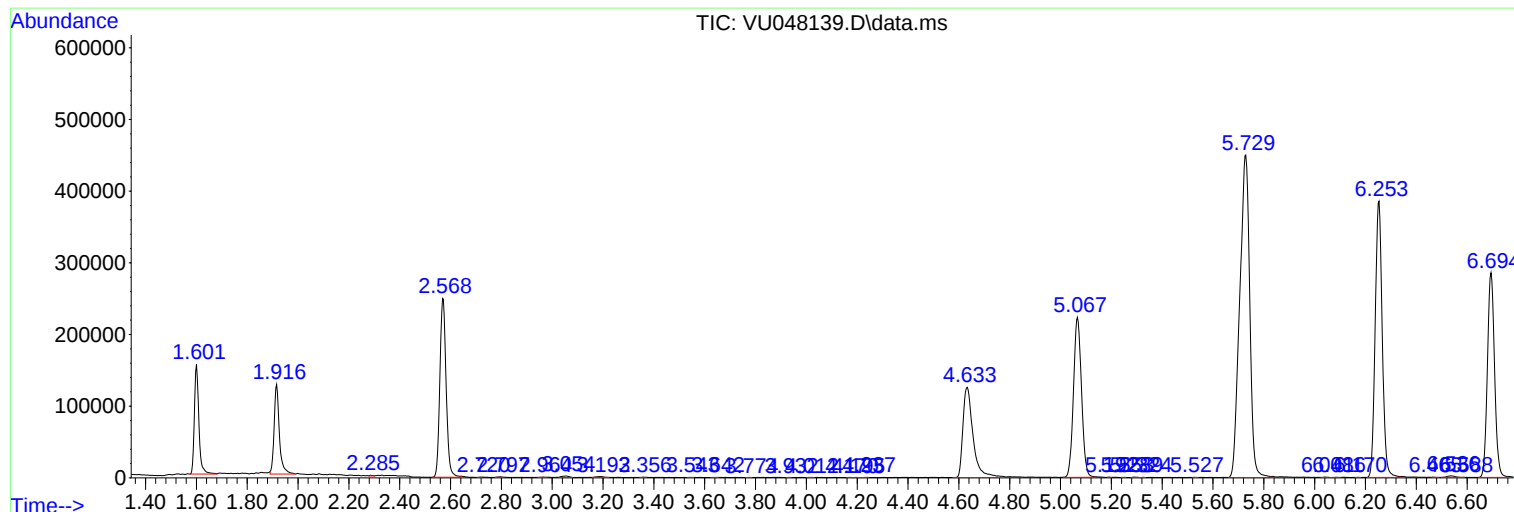

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048139.D
Acq On : 20 Apr 2022 13:51
Operator : SY/MD
Sample : VU0420WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048139.D
Acq On : 20 Apr 2022 13:51
Operator : SY/MD
Sample : VU0420WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc