

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048141.D
 Acq On : 20 Apr 2022 14:37
 Operator : SY/MD
 Sample : N2485-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rBV	147527	173877	14.94%	1.819%
2	1.916	171	179	199	rVB	115631	161891	13.91%	1.694%
3	2.568	370	382	395	rBV	252958	416442	35.78%	4.357%
4	2.732	430	433	434	rBV	321	192	0.02%	0.002%
5	2.912	484	489	495	rVB3	456	444	0.04%	0.005%
6	3.044	525	530	535	rBV5	634	811	0.07%	0.008%
7	3.083	540	542	546	rVB	186	79	0.01%	0.001%
8	3.189	565	575	585	rVB5	1010	2188	0.19%	0.023%
9	3.231	585	588	590	rBV2	188	152	0.01%	0.002%
10	3.334	618	620	623	rBV	134	74	0.01%	0.001%
11	3.446	652	655	658	rBV2	348	261	0.02%	0.003%
12	3.517	672	677	680	rBV2	384	275	0.02%	0.003%
13	3.613	704	707	711	rBV2	154	92	0.01%	0.001%
14	3.781	753	759	760	rBV2	106	91	0.01%	0.001%
15	3.842	774	778	784	rVB3	456	453	0.04%	0.005%
16	3.877	785	789	792	rBV3	171	145	0.01%	0.002%
17	3.977	818	820	825	rVB2	251	157	0.01%	0.002%
18	4.012	825	831	834	rBV2	152	175	0.02%	0.002%
19	4.031	834	837	841	rVB2	261	200	0.02%	0.002%
20	4.064	843	847	848	rBV	112	82	0.01%	0.001%
21	4.076	848	851	852	rBV2	269	157	0.01%	0.002%
22	4.134	867	869	870	rBV	164	70	0.01%	0.001%
23	4.205	888	891	893	rBV2	276	137	0.01%	0.001%
24	4.298	917	920	921	rBV	185	80	0.01%	0.001%
25	4.398	948	951	956	rBB2	331	273	0.02%	0.003%
26	4.424	956	959	965	rVB2	134	145	0.01%	0.002%
27	4.456	965	969	970	rBV	281	118	0.01%	0.001%
28	4.536	992	994	995	rBV	167	77	0.01%	0.001%
29	4.623	1008	1021	1062	rBV	124282	313564	26.94%	3.280%
30	5.067	1142	1159	1180	rBV	213653	470803	40.45%	4.925%
31	5.218	1203	1206	1209	rVB2	475	301	0.03%	0.003%
32	5.295	1223	1230	1234	rBV3	657	966	0.08%	0.010%
33	5.350	1244	1247	1249	rBV	147	97	0.01%	0.001%
34	5.395	1258	1261	1267	rVB	289	251	0.02%	0.003%
35	5.424	1268	1270	1273	rBV	100	72	0.01%	0.001%
36	5.440	1273	1275	1280	rVB2	258	129	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048141.D
 Acq On : 20 Apr 2022 14:37
 Operator : SY/MD
 Sample : N2485-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.620	1329	1331	1333	rBV	137	83	0.01%	0.001%
38	5.649	1338	1340	1343	rVB2	205	112	0.01%	0.001%
39	5.726	1343	1364	1395	rBV2	426335	1163894	100.00%	12.176%
40	6.073	1469	1472	1474	rBV2	289	189	0.02%	0.002%
41	6.125	1481	1488	1492	rBV3	392	549	0.05%	0.006%
42	6.250	1512	1527	1550	rBV	393028	751974	64.61%	7.867%
43	6.533	1607	1615	1620	rBV5	2091	3388	0.29%	0.035%
44	6.581	1628	1630	1634	rVB4	446	274	0.02%	0.003%
45	6.690	1650	1664	1685	rBV2	268365	527377	45.31%	5.517%
46	6.858	1715	1716	1720	rBV2	172	110	0.01%	0.001%
47	6.874	1720	1721	1723	rBV2	286	116	0.01%	0.001%
48	6.916	1732	1734	1737	rVB2	242	102	0.01%	0.001%
49	7.137	1801	1803	1806	rBV2	221	135	0.01%	0.001%
50	7.186	1810	1818	1829	rVV3	2827	3971	0.34%	0.042%
51	7.240	1832	1835	1841	rVB	213	171	0.01%	0.002%
52	7.276	1841	1846	1848	rBV2	174	162	0.01%	0.002%
53	7.308	1854	1856	1861	rVB2	225	116	0.01%	0.001%
54	7.340	1861	1866	1870	rBV2	318	293	0.03%	0.003%
55	7.366	1871	1874	1880	rVB2	276	223	0.02%	0.002%
56	7.459	1900	1903	1904	rBV	222	141	0.01%	0.001%
57	7.565	1922	1936	1960	rBV	134915	243699	20.94%	2.550%
58	7.694	1965	1976	1986	rVB4	1813	3273	0.28%	0.034%
59	7.797	2000	2008	2009	rBV	880	874	0.08%	0.009%
60	7.899	2023	2040	2056	rBV	513193	892926	76.72%	9.342%
61	8.182	2116	2128	2144	rBV	95987	166678	14.32%	1.744%
62	8.584	2251	2253	2255	rBV	203	102	0.01%	0.001%
63	8.633	2256	2268	2301	rBV	365340	687556	59.07%	7.193%
64	8.957	2366	2369	2371	rBB2	205	108	0.01%	0.001%
65	8.986	2376	2378	2380	rBV2	293	102	0.01%	0.001%
66	9.015	2385	2387	2389	rBV2	271	179	0.02%	0.002%
67	9.073	2402	2405	2409	rBV2	308	192	0.02%	0.002%
68	9.285	2468	2471	2472	rBV	321	127	0.01%	0.001%
69	9.311	2477	2479	2482	rVB	198	94	0.01%	0.001%
70	9.362	2493	2495	2498	rVB	307	143	0.01%	0.001%
71	9.417	2498	2512	2550	rBV	588951	1008431	86.64%	10.550%
72	9.568	2556	2559	2563	rBV2	542	439	0.04%	0.005%
73	9.639	2577	2581	2589	rBV3	224	308	0.03%	0.003%
74	9.697	2591	2599	2604	rBV3	760	940	0.08%	0.010%
75	9.867	2649	2652	2653	rBV	196	88	0.01%	0.001%
76	9.903	2660	2663	2665	rBV2	115	78	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048141.D
 Acq On : 20 Apr 2022 14:37
 Operator : SY/MD
 Sample : N2485-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COHX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.960	2678	2681	2682	rBV	151	97	0.01%	0.001%
78	10.044	2704	2707	2709	rBV	136	85	0.01%	0.001%
79	10.089	2717	2721	2723	rBV2	264	236	0.02%	0.002%
80	10.134	2733	2735	2738	rVB2	234	102	0.01%	0.001%
81	10.176	2745	2748	2751	rBV2	234	131	0.01%	0.001%
82	10.240	2763	2768	2773	rBV3	773	798	0.07%	0.008%
83	10.288	2781	2783	2788	rBV2	261	213	0.02%	0.002%
84	10.327	2792	2795	2798	rBV	258	185	0.02%	0.002%
85	10.353	2798	2803	2806	rBV3	830	682	0.06%	0.007%
86	10.398	2814	2817	2819	rBV	257	151	0.01%	0.002%
87	10.488	2841	2845	2852	rBV2	277	283	0.02%	0.003%
88	10.571	2864	2871	2876	rBV4	1195	1486	0.13%	0.016%
89	10.671	2896	2902	2909	rVB3	2406	2827	0.24%	0.030%
90	10.758	2915	2929	2948	rBV	410090	651996	56.02%	6.821%
91	11.462	3140	3148	3150	rBV4	1552	1984	0.17%	0.021%
92	11.575	3180	3183	3189	rVB3	379	386	0.03%	0.004%
93	11.639	3201	3203	3205	rBV	255	122	0.01%	0.001%
94	11.812	3244	3257	3275	rBV	624395	992989	85.32%	10.388%
95	12.066	3328	3336	3346	rBV3	9621	15016	1.29%	0.157%
96	12.192	3363	3375	3396	rVB	535984	875931	75.26%	9.164%
97	12.767	3550	3554	3557	rBV3	799	796	0.07%	0.008%
98	12.854	3579	3581	3582	rBV	306	134	0.01%	0.001%
99	12.893	3587	3593	3600	rVV5	4474	6348	0.55%	0.066%
100	12.967	3612	3616	3620	rBV3	556	659	0.06%	0.007%




Sum of corrected areas: 9558675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048141.D
Acq On : 20 Apr 2022 14:37
Operator : SY/MD
Sample : N2485-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

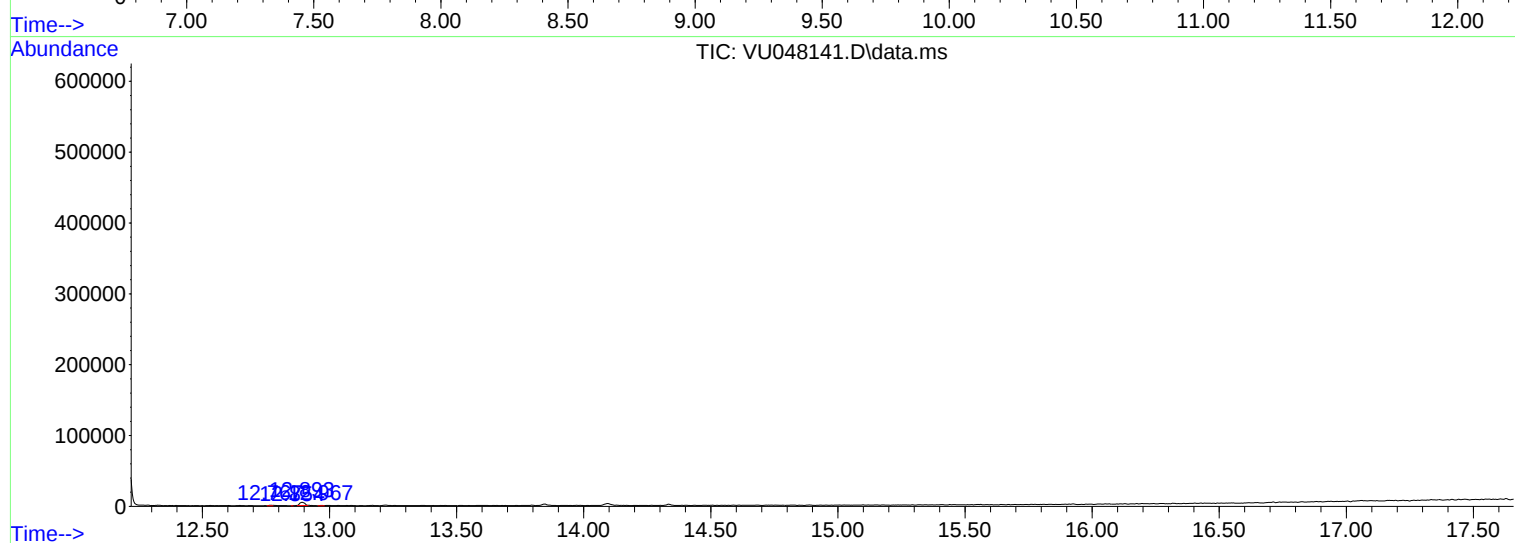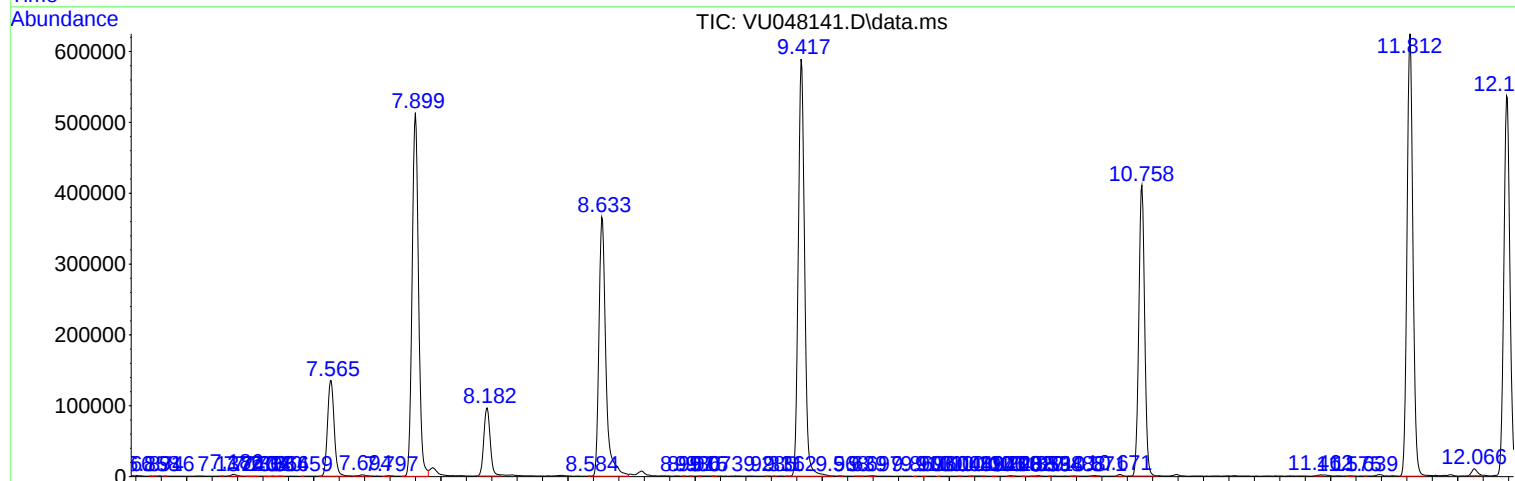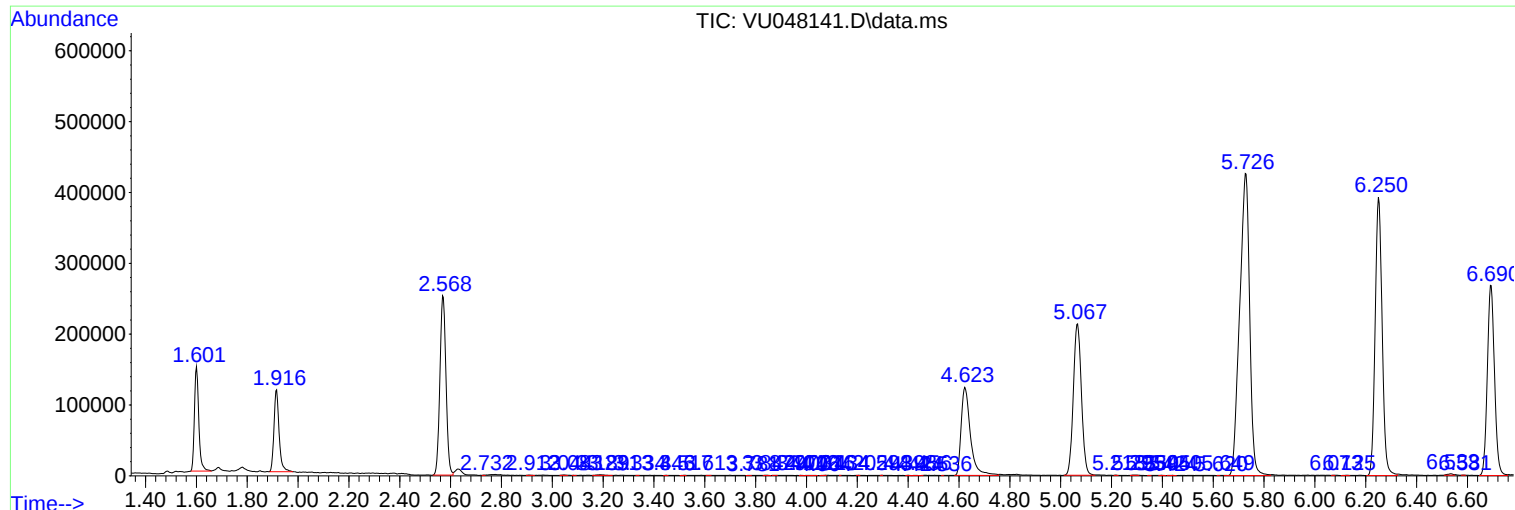

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048141.D
Acq On : 20 Apr 2022 14:37
Operator : SY/MD
Sample : N2485-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048141.D
Acq On : 20 Apr 2022 14:37
Operator : SY/MD
Sample : N2485-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HX8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------