

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048143.D
 Acq On : 20 Apr 2022 15:23
 Operator : SY/MD
 Sample : N2485-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	147658	173980	15.09%	1.838%
2	1.916	170	179	197	rBV	112524	156782	13.59%	1.656%
3	2.568	370	382	395	rBV	234638	385713	33.45%	4.074%
4	2.697	419	422	424	rVB3	411	178	0.02%	0.002%
5	2.765	440	443	447	rVV3	414	340	0.03%	0.004%
6	2.787	447	450	453	rVV4	262	193	0.02%	0.002%
7	2.829	461	463	468	rBV2	277	239	0.02%	0.003%
8	2.961	497	504	507	rBV3	472	652	0.06%	0.007%
9	2.996	512	515	520	rVB	454	365	0.03%	0.004%
10	3.051	527	532	539	rVB5	654	783	0.07%	0.008%
11	3.189	567	575	584	rVB4	858	1655	0.14%	0.017%
12	3.234	584	589	591	rBV	178	202	0.02%	0.002%
13	3.273	599	601	607	rVB2	332	290	0.03%	0.003%
14	3.433	647	651	656	rVV3	290	303	0.03%	0.003%
15	3.475	659	664	667	rBV3	235	235	0.02%	0.002%
16	3.530	677	681	685	rVB2	264	222	0.02%	0.002%
17	3.562	685	691	694	rBV2	218	236	0.02%	0.002%
18	3.642	712	716	722	rVB2	210	197	0.02%	0.002%
19	3.707	730	736	741	rVB3	268	336	0.03%	0.004%
20	3.900	793	796	800	rVB2	249	185	0.02%	0.002%
21	3.945	808	810	814	rVB2	314	198	0.02%	0.002%
22	4.211	887	893	896	rBV3	321	350	0.03%	0.004%
23	4.456	965	969	973	rBV2	285	240	0.02%	0.003%
24	4.482	974	977	981	rVB	281	216	0.02%	0.002%
25	4.555	994	1000	1004	rVB2	315	271	0.02%	0.003%
26	4.623	1004	1021	1055	rBV2	123050	314291	27.25%	3.320%
27	4.919	1110	1113	1116	rVB2	294	202	0.02%	0.002%
28	4.941	1116	1120	1126	rBV2	292	350	0.03%	0.004%
29	5.067	1141	1159	1182	rBV	212822	467648	40.55%	4.940%
30	5.179	1192	1194	1200	rBV4	280	237	0.02%	0.003%
31	5.282	1221	1226	1228	rBV2	377	328	0.03%	0.003%
32	5.443	1273	1276	1280	rVB2	259	195	0.02%	0.002%
33	5.617	1323	1330	1335	rBV2	222	246	0.02%	0.003%
34	5.726	1342	1364	1391	rBV2	422553	1153244	100.00%	12.182%
35	6.096	1476	1479	1481	rBV3	299	225	0.02%	0.002%
36	6.131	1487	1490	1494	rBV2	353	303	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048143.D
 Acq On : 20 Apr 2022 15:23
 Operator : SY/MD
 Sample : N2485-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1510	1527	1559	rBV	386003	747563	64.82%	7.896%
38	6.533	1607	1615	1625	rBV7	2048	3700	0.32%	0.039%
39	6.575	1626	1628	1631	rVV3	706	297	0.03%	0.003%
40	6.600	1631	1636	1639	rVB4	395	414	0.04%	0.004%
41	6.694	1650	1665	1687	rVV	270946	528331	45.81%	5.581%
42	6.809	1699	1701	1706	rVB3	506	330	0.03%	0.003%
43	6.893	1724	1727	1731	rVB2	456	317	0.03%	0.003%
44	7.018	1760	1766	1767	rBV	189	186	0.02%	0.002%
45	7.112	1789	1795	1799	rBV	275	193	0.02%	0.002%
46	7.137	1799	1803	1807	rBV2	464	384	0.03%	0.004%
47	7.186	1811	1818	1825	rBV3	2606	4017	0.35%	0.042%
48	7.234	1829	1833	1836	rBV	265	239	0.02%	0.003%
49	7.311	1851	1857	1861	rBV2	180	217	0.02%	0.002%
50	7.465	1900	1905	1909	rBV2	220	273	0.02%	0.003%
51	7.565	1923	1936	1961	rBV	133091	239651	20.78%	2.531%
52	7.690	1967	1975	1985	rVB4	1820	2992	0.26%	0.032%
53	7.735	1985	1989	1991	rVB2	428	328	0.03%	0.003%
54	7.787	2002	2005	2006	rBV	383	193	0.02%	0.002%
55	7.899	2025	2040	2056	rBV	517292	885105	76.75%	9.349%
56	8.179	2116	2127	2148	rBV	94181	164865	14.30%	1.741%
57	8.378	2187	2189	2193	rVB2	287	182	0.02%	0.002%
58	8.407	2196	2198	2203	rVB3	255	217	0.02%	0.002%
59	8.440	2206	2208	2212	rBV	300	203	0.02%	0.002%
60	8.472	2213	2218	2227	rVB2	633	1020	0.09%	0.011%
61	8.523	2232	2234	2237	rVB	350	229	0.02%	0.002%
62	8.542	2237	2240	2243	rBV2	317	269	0.02%	0.003%
63	8.636	2256	2269	2302	rBV	349560	666567	57.80%	7.041%
64	8.790	2311	2317	2333	rVB7	4549	8488	0.74%	0.090%
65	8.899	2348	2351	2356	rBV3	319	318	0.03%	0.003%
66	8.928	2356	2360	2361	rBV2	394	251	0.02%	0.003%
67	9.018	2385	2388	2393	rBV2	313	299	0.03%	0.003%
68	9.057	2397	2400	2405	rVB2	350	243	0.02%	0.003%
69	9.086	2405	2409	2411	rBV2	383	254	0.02%	0.003%
70	9.214	2445	2449	2451	rBV	276	183	0.02%	0.002%
71	9.417	2498	2512	2551	rBV	582147	1001590	86.85%	10.580%
72	9.690	2591	2597	2598	rBV2	699	565	0.05%	0.006%
73	9.954	2675	2679	2682	rVB2	264	178	0.02%	0.002%
74	10.349	2795	2802	2804	rBV	617	622	0.05%	0.007%
75	10.626	2885	2888	2891	rBV2	225	181	0.02%	0.002%
76	10.671	2895	2902	2911	rVB4	2184	3016	0.26%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048143.D
 Acq On : 20 Apr 2022 15:23
 Operator : SY/MD
 Sample : N2485-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.758	2916	2929	2947	rBV	387801	631521	54.76%	6.671%
78	10.893	2959	2971	2975	rBV3	1202	1784	0.15%	0.019%
79	11.353	3111	3114	3117	rBV	246	210	0.02%	0.002%
80	11.465	3139	3149	3158	rBV10	1592	3133	0.27%	0.033%
81	11.690	3213	3219	3228	rBV6	1573	2376	0.21%	0.025%
82	11.745	3233	3236	3240	rBV3	385	377	0.03%	0.004%
83	11.812	3244	3257	3283	rVV	616352	979704	84.95%	10.348%
84	11.928	3289	3293	3295	rBV3	662	503	0.04%	0.005%
85	12.063	3326	3335	3348	rBV2	16138	27880	2.42%	0.294%
86	12.195	3359	3376	3394	rBV	530984	879711	76.28%	9.292%
87	12.324	3412	3416	3420	rVB4	488	451	0.04%	0.005%
88	12.436	3447	3451	3453	rBV2	306	288	0.02%	0.003%
89	12.475	3460	3463	3466	rBV3	518	310	0.03%	0.003%
90	12.494	3466	3469	3472	rBV2	333	301	0.03%	0.003%
91	12.536	3479	3482	3485	rBV2	325	184	0.02%	0.002%
92	12.607	3501	3504	3507	rBV2	249	178	0.02%	0.002%
93	12.754	3544	3550	3552	rBV3	308	303	0.03%	0.003%
94	12.774	3552	3556	3559	rVV	422	369	0.03%	0.004%
95	12.893	3585	3593	3602	rBV6	4501	5974	0.52%	0.063%
96	12.976	3617	3619	3622	rBV	286	193	0.02%	0.002%
97	13.140	3667	3670	3674	rBV3	328	309	0.03%	0.003%
98	13.224	3692	3696	3700	rBV2	428	447	0.04%	0.005%
99	13.844	3883	3889	3899	rVB7	1785	2414	0.21%	0.025%
100	14.095	3963	3967	3978	rVB5	1660	2142	0.19%	0.023%




Sum of corrected areas: 9467162

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048143.D
Acq On : 20 Apr 2022 15:23
Operator : SY/MD
Sample : N2485-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

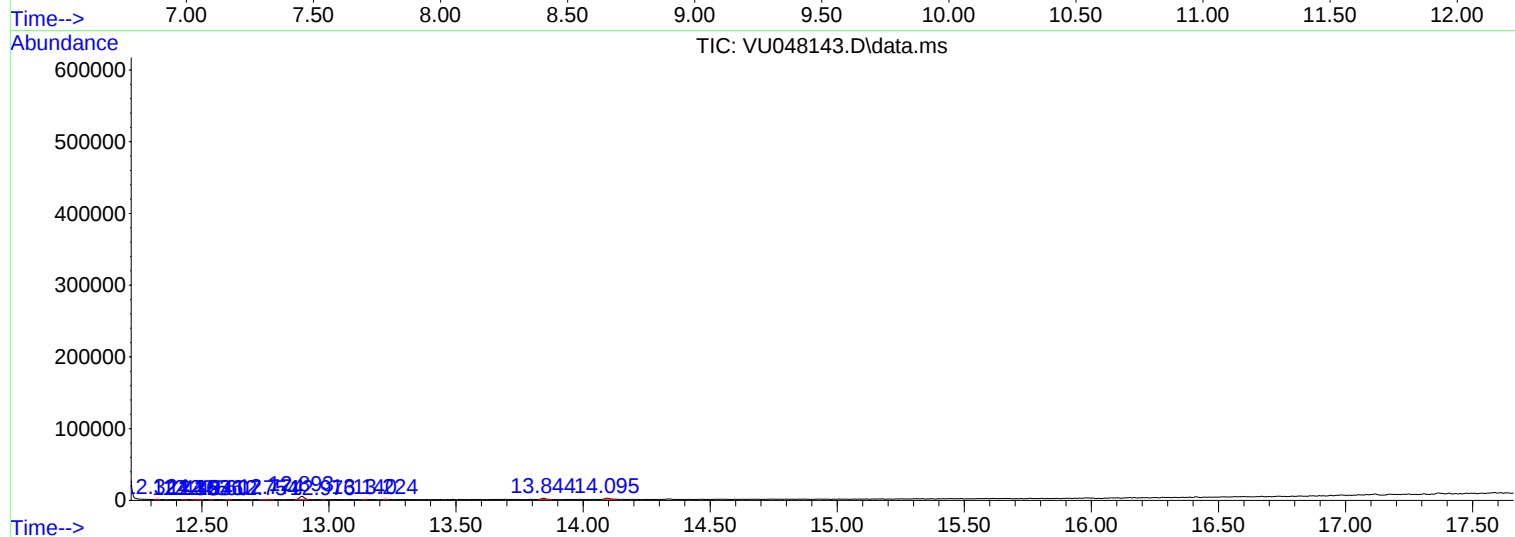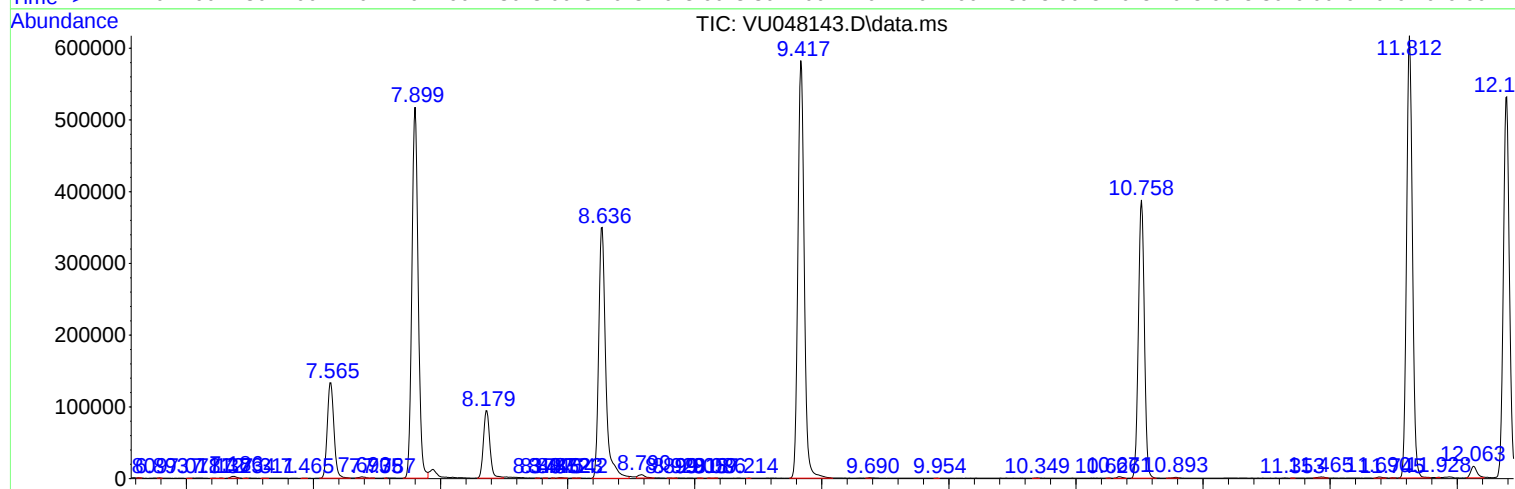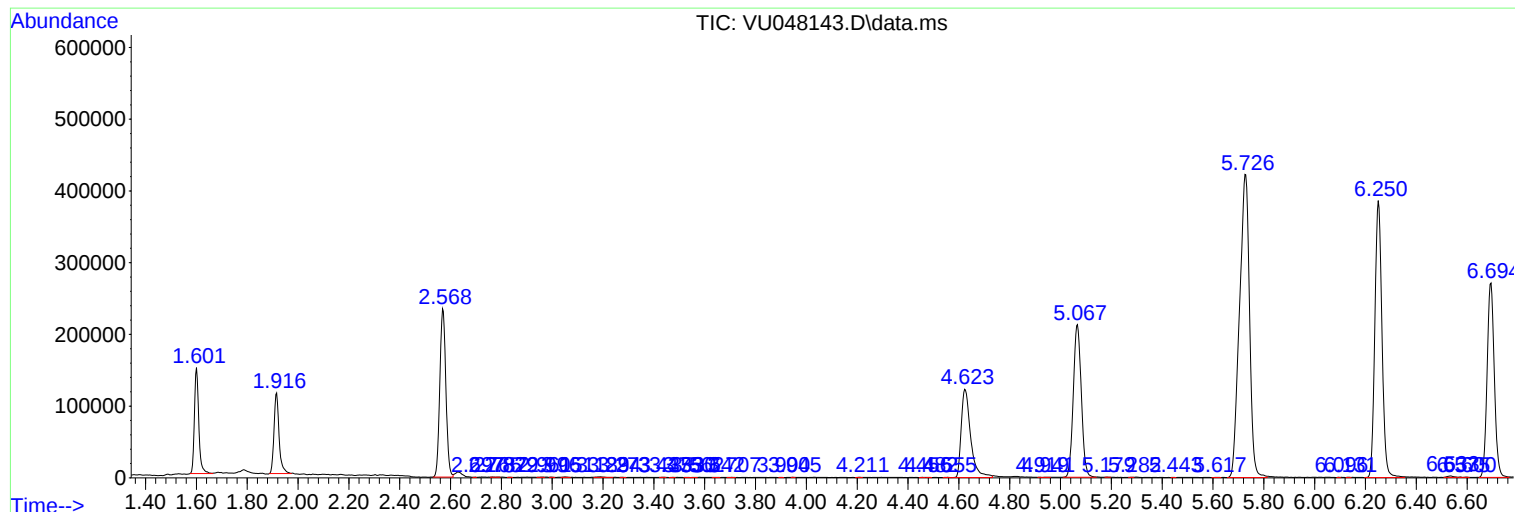

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048143.D
Acq On : 20 Apr 2022 15:23
Operator : SY/MD
Sample : N2485-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048143.D
Acq On : 20 Apr 2022 15:23
Operator : SY/MD
Sample : N2485-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc