

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048144.D
 Acq On : 20 Apr 2022 15:46
 Operator : SY/MD
 Sample : N2485-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rBV	146241	172892	14.58%	1.762%
2	1.916	171	179	202	rVB	115938	166208	14.02%	1.694%
3	2.571	370	383	396	rBV	250979	412978	34.83%	4.209%
4	2.674	413	415	420	rBV2	376	267	0.02%	0.003%
5	2.838	464	466	470	rVB	230	170	0.01%	0.002%
6	2.957	497	503	506	rBV	394	340	0.03%	0.003%
7	3.022	522	523	526	rVV2	274	175	0.01%	0.002%
8	3.054	526	533	538	rVB6	784	1018	0.09%	0.010%
9	3.096	544	546	549	rVB2	228	104	0.01%	0.001%
10	3.141	557	560	562	rBV	283	155	0.01%	0.002%
11	3.186	562	574	590	rVB	5874	12859	1.08%	0.131%
12	3.247	590	593	596	rBV	319	221	0.02%	0.002%
13	3.266	596	599	600	rBV3	231	132	0.01%	0.001%
14	3.362	616	629	641	rBV4	3354	7192	0.61%	0.073%
15	3.549	682	687	690	rBV2	359	333	0.03%	0.003%
16	3.652	714	719	722	rBV2	137	141	0.01%	0.001%
17	3.674	723	726	732	rVV3	260	277	0.02%	0.003%
18	3.758	748	752	755	rBV	147	135	0.01%	0.001%
19	3.780	755	759	761	rVV	183	134	0.01%	0.001%
20	3.793	761	763	767	rVV2	220	113	0.01%	0.001%
21	3.813	767	769	777	rVB2	249	199	0.02%	0.002%
22	3.903	794	797	800	rVB	190	126	0.01%	0.001%
23	3.951	806	812	818	rVB3	267	239	0.02%	0.002%
24	3.986	820	823	828	rBV	236	136	0.01%	0.001%
25	4.012	828	831	834	rBV	225	113	0.01%	0.001%
26	4.031	834	837	839	rBV2	227	131	0.01%	0.001%
27	4.102	857	859	861	rBV	225	103	0.01%	0.001%
28	4.153	870	875	879	rBV2	103	135	0.01%	0.001%
29	4.182	879	884	887	rBV2	228	179	0.02%	0.002%
30	4.243	899	903	905	rBV2	149	106	0.01%	0.001%
31	4.311	922	924	927	rBV	214	131	0.01%	0.001%
32	4.375	941	944	949	rBV2	203	203	0.02%	0.002%
33	4.436	960	963	967	rBV	225	149	0.01%	0.002%
34	4.485	975	978	981	rBV2	139	128	0.01%	0.001%
35	4.539	992	995	999	rVB	173	125	0.01%	0.001%
36	4.562	999	1002	1007	rBV2	231	252	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048144.D
 Acq On : 20 Apr 2022 15:46
 Operator : SY/MD
 Sample : N2485-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	4.620	1007	1020	1052	rBV	122625	306298	25.83%	3.122%
38	5.067	1142	1159	1193	rVB	213462	470287	39.66%	4.793%
39	5.218	1202	1206	1208	rBV3	486	369	0.03%	0.004%
40	5.259	1214	1219	1220	rBV	355	259	0.02%	0.003%
41	5.333	1238	1242	1243	rBV2	176	138	0.01%	0.001%
42	5.369	1251	1253	1258	rVB2	300	205	0.02%	0.002%
43	5.446	1272	1277	1283	rBV2	188	237	0.02%	0.002%
44	5.517	1296	1299	1304	rBV	182	127	0.01%	0.001%
45	5.591	1319	1322	1326	rBV	215	166	0.01%	0.002%
46	5.729	1336	1365	1377	rBV2	429567	1185859	100.00%	12.087%
47	6.021	1454	1456	1459	rVB2	290	186	0.02%	0.002%
48	6.044	1459	1463	1467	rBV2	505	443	0.04%	0.005%
49	6.060	1467	1468	1471	rVB	307	134	0.01%	0.001%
50	6.083	1471	1475	1477	rBV	213	174	0.01%	0.002%
51	6.157	1495	1498	1501	rBV3	277	217	0.02%	0.002%
52	6.195	1506	1510	1513	rBV3	315	264	0.02%	0.003%
53	6.250	1513	1527	1563	rVV	399266	756893	63.83%	7.715%
54	6.536	1607	1616	1627	rBV6	1645	2959	0.25%	0.030%
55	6.693	1647	1665	1688	rBV	271069	534533	45.08%	5.448%
56	6.790	1694	1695	1700	rBV	384	261	0.02%	0.003%
57	7.009	1759	1763	1766	rBV	289	154	0.01%	0.002%
58	7.041	1770	1773	1781	rVB2	314	371	0.03%	0.004%
59	7.105	1790	1793	1795	rBV2	181	106	0.01%	0.001%
60	7.182	1810	1817	1829	rBV2	2452	4039	0.34%	0.041%
61	7.230	1829	1832	1835	rVV	327	194	0.02%	0.002%
62	7.298	1850	1853	1857	rVB2	299	191	0.02%	0.002%
63	7.330	1857	1863	1866	rBV	243	268	0.02%	0.003%
64	7.353	1866	1870	1876	rVV2	290	246	0.02%	0.003%
65	7.385	1877	1880	1884	rVB2	184	130	0.01%	0.001%
66	7.565	1924	1936	1957	rBV	135262	243207	20.51%	2.479%
67	7.738	1988	1990	1995	rVB3	324	191	0.02%	0.002%
68	7.793	2004	2007	2009	rBV3	408	261	0.02%	0.003%
69	7.851	2021	2025	2026	rBV	382	267	0.02%	0.003%
70	7.899	2026	2040	2056	rBV	510857	896009	75.56%	9.133%
71	8.124	2108	2110	2112	rBV2	192	106	0.01%	0.001%
72	8.179	2115	2127	2142	rBV	96923	165887	13.99%	1.691%
73	8.632	2256	2268	2300	rBV	351639	679954	57.34%	6.931%
74	8.918	2355	2357	2365	rVB3	307	275	0.02%	0.003%
75	8.973	2371	2374	2380	rVB	228	181	0.02%	0.002%
76	9.217	2447	2450	2454	rBV2	316	251	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048144.D
 Acq On : 20 Apr 2022 15:46
 Operator : SY/MD
 Sample : N2485-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	9.275	2464	2468	2470	rBV2	250	175	0.01%	0.002%
78	9.333	2483	2486	2487	rBV	190	114	0.01%	0.001%
79	9.417	2498	2512	2553	rBV	601407	1146767	96.70%	11.689%
80	9.635	2577	2580	2582	rBV2	150	106	0.01%	0.001%
81	9.697	2591	2599	2604	rBV3	664	953	0.08%	0.010%
82	9.745	2611	2614	2616	rBV2	222	140	0.01%	0.001%
83	10.317	2789	2792	2794	rBV	234	125	0.01%	0.001%
84	10.385	2809	2813	2815	rBV2	151	139	0.01%	0.001%
85	10.420	2822	2824	2827	rBV	284	150	0.01%	0.002%
86	10.635	2887	2891	2894	rBV2	221	253	0.02%	0.003%
87	10.671	2895	2902	2911	rVB5	2002	3141	0.26%	0.032%
88	10.758	2916	2929	2948	rVV	414745	671424	56.62%	6.844%
89	10.844	2953	2956	2957	rBV	260	131	0.01%	0.001%
90	11.073	3022	3027	3029	rBV2	364	379	0.03%	0.004%
91	11.452	3140	3145	3146	rBV3	1189	934	0.08%	0.010%
92	11.748	3230	3237	3244	rBV4	2427	3300	0.28%	0.034%
93	11.812	3244	3257	3280	rBV	614662	1044209	88.06%	10.643%
94	12.195	3362	3376	3394	rBV	522947	906091	76.41%	9.235%
95	12.368	3428	3430	3436	rBV2	311	284	0.02%	0.003%
96	12.397	3437	3439	3442	rBV	441	223	0.02%	0.002%
97	12.446	3450	3454	3457	rBV2	314	317	0.03%	0.003%
98	12.494	3466	3469	3476	rVB3	373	420	0.04%	0.004%
99	12.526	3476	3479	3482	rBV2	388	310	0.03%	0.003%
100	12.944	3606	3609	3612	rBV2	341	280	0.02%	0.003%




Sum of corrected areas: 9810961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048144.D
Acq On : 20 Apr 2022 15:46
Operator : SY/MD
Sample : N2485-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

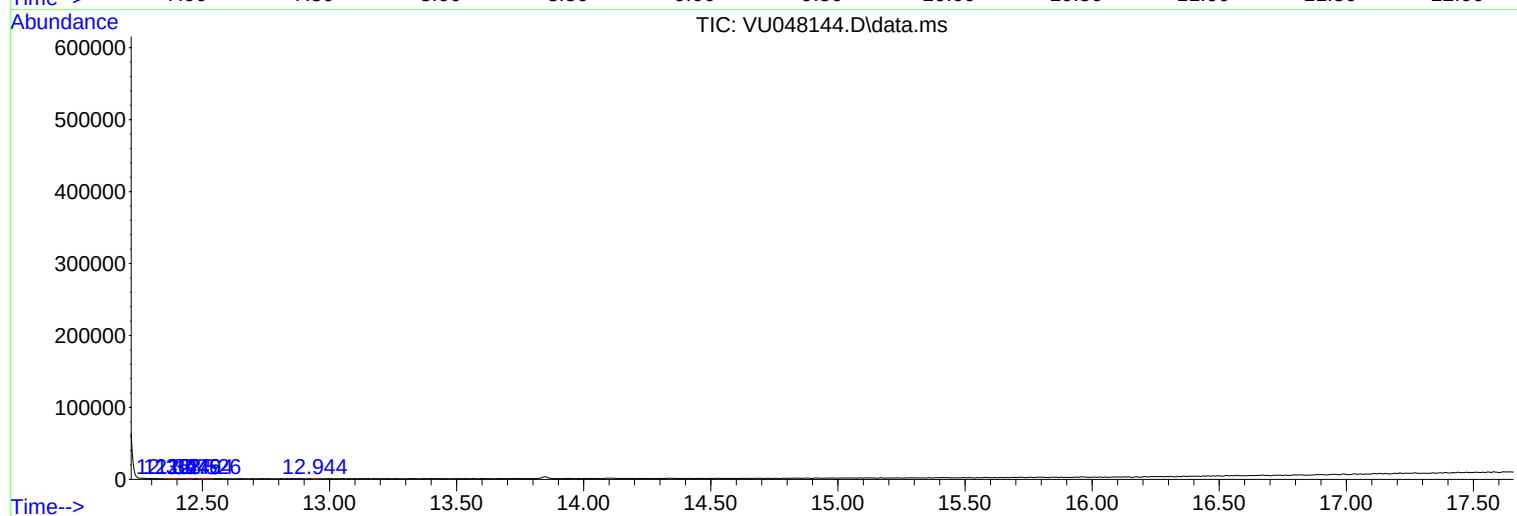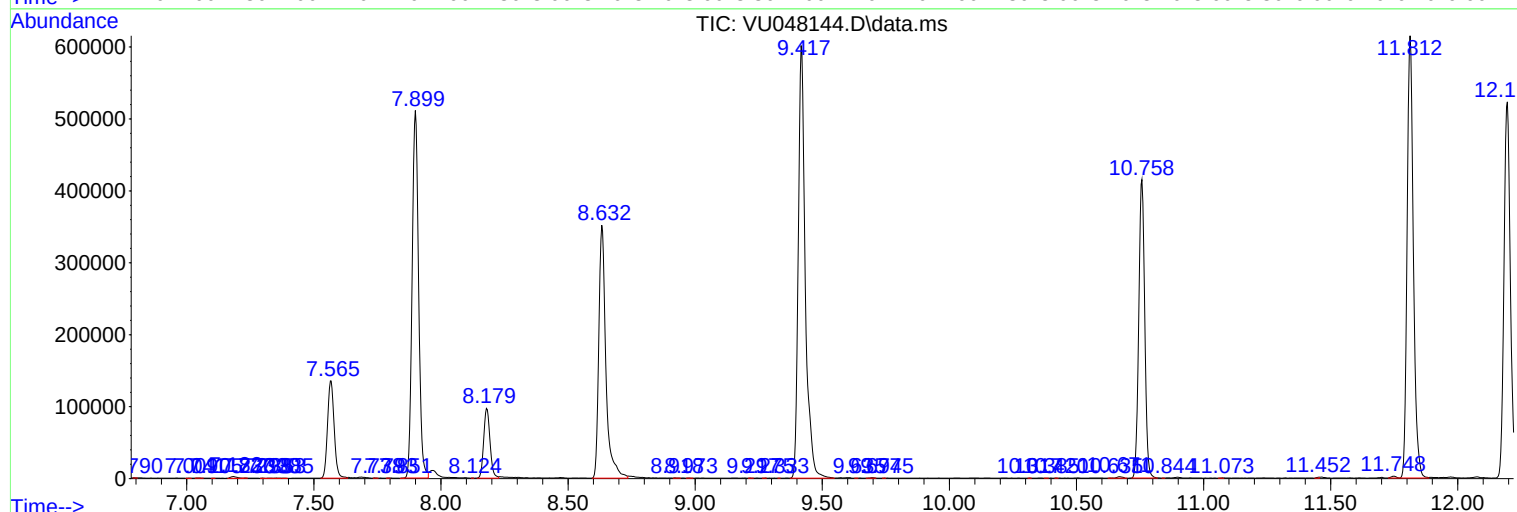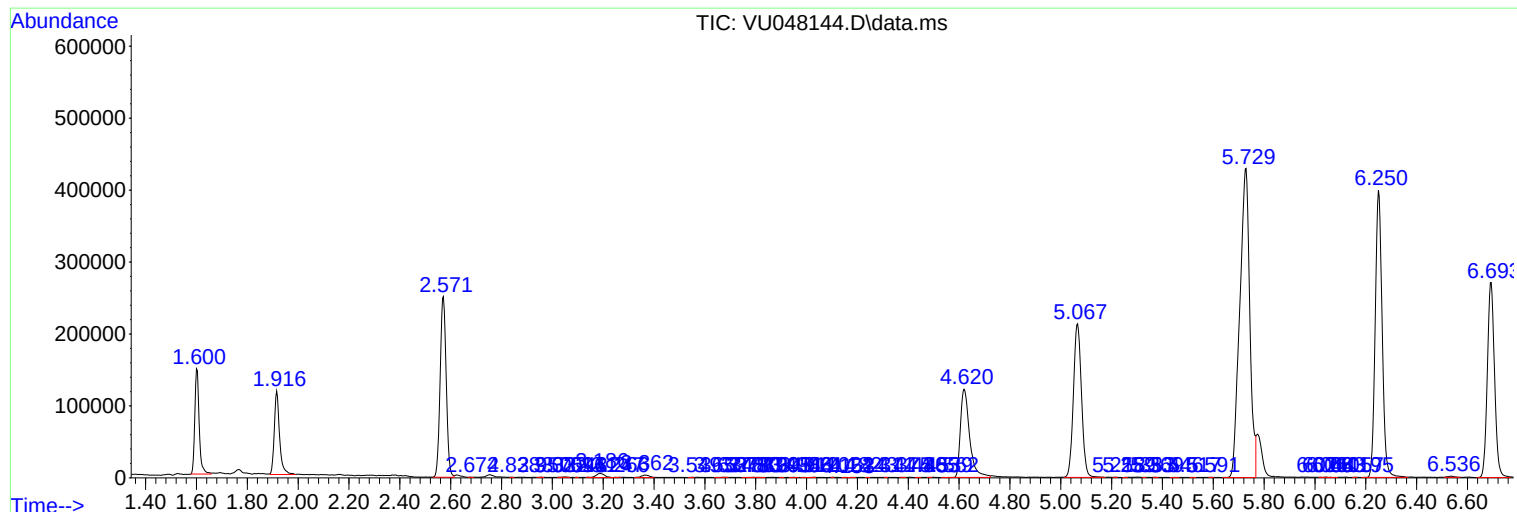

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048144.D
Acq On : 20 Apr 2022 15:46
Operator : SY/MD
Sample : N2485-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048144.D
Acq On : 20 Apr 2022 15:46
Operator : SY/MD
Sample : N2485-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc