

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048146.D
 Acq On : 20 Apr 2022 16:32
 Operator : SY/MD
 Sample : N2485-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	19	rVB3	19116	20942	1.70%	0.215%
2	1.491	42	47	53	rBV3	4922	6547	0.53%	0.067%
3	1.600	73	81	96	rBV	155323	188659	15.28%	1.938%
4	1.916	171	179	197	rVB	111175	156372	12.66%	1.606%
5	2.572	370	383	397	rBV	245054	403209	32.66%	4.142%
6	2.687	415	419	420	rBV2	323	235	0.02%	0.002%
7	2.755	435	440	442	rBV4	1798	1568	0.13%	0.016%
8	2.916	482	490	493	rVB3	234	332	0.03%	0.003%
9	2.983	507	511	516	rVB4	475	516	0.04%	0.005%
10	3.047	523	531	536	rBV4	943	1472	0.12%	0.015%
11	3.189	564	575	589	rBV2	3599	7942	0.64%	0.082%
12	3.362	623	629	634	rBV3	1071	1558	0.13%	0.016%
13	3.433	646	651	653	rBV	393	355	0.03%	0.004%
14	3.555	685	689	692	rBV4	408	353	0.03%	0.004%
15	3.687	726	730	731	rBV3	704	531	0.04%	0.005%
16	3.703	733	735	743	rVB5	1082	1049	0.08%	0.011%
17	3.870	785	787	794	rVV2	347	368	0.03%	0.004%
18	3.928	797	805	808	rBV2	435	522	0.04%	0.005%
19	4.346	931	935	941	rVB2	426	407	0.03%	0.004%
20	4.382	941	946	948	rBV	268	197	0.02%	0.002%
21	4.623	1008	1021	1056	rBV	121277	304905	24.69%	3.132%
22	5.067	1142	1159	1181	rVV	208698	458581	37.14%	4.711%
23	5.163	1187	1189	1201	rVB4	765	996	0.08%	0.010%
24	5.221	1201	1207	1208	rBV3	330	335	0.03%	0.003%
25	5.269	1219	1222	1224	rBV2	305	201	0.02%	0.002%
26	5.356	1244	1249	1251	rVV2	227	201	0.02%	0.002%
27	5.385	1255	1258	1263	rVB2	256	212	0.02%	0.002%
28	5.449	1276	1278	1284	rBV2	276	242	0.02%	0.002%
29	5.526	1300	1302	1308	rVB4	332	321	0.03%	0.003%
30	5.591	1317	1322	1324	rBV3	306	224	0.02%	0.002%
31	5.726	1343	1364	1372	rBV2	416081	1123559	91.00%	11.542%
32	6.099	1476	1480	1483	rBV3	559	555	0.04%	0.006%
33	6.140	1490	1493	1497	rBV2	492	492	0.04%	0.005%
34	6.250	1512	1527	1547	rBV	325658	623016	50.46%	6.400%
35	6.530	1606	1614	1619	rBV3	1385	2146	0.17%	0.022%
36	6.690	1650	1664	1691	rBV	262406	515242	41.73%	5.293%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048146.D
 Acq On : 20 Apr 2022 16:32
 Operator : SY/MD
 Sample : N2485-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.825	1704	1706	1712	rVB4	372	270	0.02%	0.003%
38	6.877	1716	1722	1725	rBV	239	243	0.02%	0.002%
39	6.903	1725	1730	1734	rVB	198	204	0.02%	0.002%
40	7.047	1770	1775	1780	rBV2	478	440	0.04%	0.005%
41	7.185	1811	1818	1827	rVV3	2100	3365	0.27%	0.035%
42	7.507	1916	1918	1923	rVB	370	251	0.02%	0.003%
43	7.568	1923	1937	1959	rBV2	130736	235661	19.09%	2.421%
44	7.687	1968	1974	1975	rBV	1040	910	0.07%	0.009%
45	7.697	1975	1977	1989	rVB5	1912	2036	0.16%	0.021%
46	7.899	2026	2040	2056	rBV	500020	870340	70.49%	8.941%
47	8.179	2115	2127	2148	rBV	93416	161673	13.09%	1.661%
48	8.420	2196	2202	2204	rBV2	209	214	0.02%	0.002%
49	8.475	2216	2219	2223	rVB2	862	552	0.04%	0.006%
50	8.510	2226	2230	2237	rVB4	463	483	0.04%	0.005%
51	8.549	2240	2242	2244	rBV3	568	339	0.03%	0.003%
52	8.632	2255	2268	2298	rBV	348193	652241	52.82%	6.700%
53	8.870	2338	2342	2344	rVV	370	256	0.02%	0.003%
54	8.909	2351	2354	2356	rBV	275	192	0.02%	0.002%
55	8.986	2375	2378	2383	rBV3	349	290	0.02%	0.003%
56	9.160	2429	2432	2437	rVV2	341	301	0.02%	0.003%
57	9.420	2499	2513	2516	rBV	508318	792888	64.22%	8.145%
58	9.597	2565	2568	2569	rBV2	428	251	0.02%	0.003%
59	9.693	2591	2598	2608	rBV5	1053	1651	0.13%	0.017%
60	9.745	2608	2614	2617	rVB3	225	228	0.02%	0.002%
61	10.021	2697	2700	2703	rVB2	260	197	0.02%	0.002%
62	10.047	2703	2708	2710	rBV2	338	271	0.02%	0.003%
63	10.105	2723	2726	2729	rVB2	422	258	0.02%	0.003%
64	10.131	2729	2734	2740	rBV2	194	265	0.02%	0.003%
65	10.340	2795	2799	2802	rBV2	229	205	0.02%	0.002%
66	10.565	2864	2869	2875	rVB3	316	348	0.03%	0.004%
67	10.674	2895	2903	2910	rBV3	1963	2472	0.20%	0.025%
68	10.758	2915	2929	2949	rVV	397158	646395	52.35%	6.640%
69	10.870	2960	2964	2966	rBV2	412	341	0.03%	0.004%
70	10.893	2966	2971	2979	rVV3	1711	2202	0.18%	0.023%
71	11.025	3009	3012	3016	rBV	408	327	0.03%	0.003%
72	11.163	3053	3055	3062	rVB	386	343	0.03%	0.004%
73	11.208	3062	3069	3072	rBV3	325	438	0.04%	0.004%
74	11.455	3142	3146	3161	rVB5	1484	2481	0.20%	0.025%
75	11.545	3170	3174	3179	rBV	308	327	0.03%	0.003%
76	11.574	3179	3183	3185	rBV2	580	355	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048146.D
 Acq On : 20 Apr 2022 16:32
 Operator : SY/MD
 Sample : N2485-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.693	3215	3220	3225	rVB4	674	708	0.06%	0.007%
78	11.745	3226	3236	3245	rBV2	29628	46469	3.76%	0.477%
79	11.812	3245	3257	3280	rVB2	527839	1106944	89.65%	11.371%
80	11.970	3303	3306	3307	rBV2	702	452	0.04%	0.005%
81	12.066	3327	3336	3350	rBV4	4682	9203	0.75%	0.095%
82	12.195	3360	3376	3398	rBV3	584414	1234731	100.00%	12.684%
83	12.401	3435	3440	3443	rBV2	282	288	0.02%	0.003%
84	12.417	3443	3445	3452	rVB3	468	428	0.03%	0.004%
85	12.471	3459	3462	3465	rBV3	363	207	0.02%	0.002%
86	12.491	3465	3468	3472	rVB2	355	250	0.02%	0.003%
87	12.513	3472	3475	3481	rBV	510	431	0.03%	0.004%
88	12.581	3492	3496	3498	rBV2	295	201	0.02%	0.002%
89	12.629	3508	3511	3516	rBV2	417	455	0.04%	0.005%
90	12.729	3538	3542	3544	rBV2	353	272	0.02%	0.003%
91	12.767	3552	3554	3558	rBV2	378	272	0.02%	0.003%
92	12.873	3582	3587	3591	rBV3	475	429	0.03%	0.004%
93	12.976	3614	3619	3623	rVB3	761	629	0.05%	0.006%
94	13.057	3639	3644	3648	rBV2	319	369	0.03%	0.004%
95	13.230	3692	3698	3702	rBV2	538	582	0.05%	0.006%
96	13.333	3728	3730	3734	rVB2	431	282	0.02%	0.003%
97	13.841	3877	3888	3905	rVB	60796	98301	7.96%	1.010%
98	14.066	3955	3958	3960	rBV	378	269	0.02%	0.003%
99	14.330	4032	4040	4053	rVB2	16845	25430	2.06%	0.261%
100	14.439	4070	4074	4075	rBV	417	278	0.02%	0.003%


Sum of corrected areas: 9734746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048146.D
Acq On : 20 Apr 2022 16:32
Operator : SY/MD
Sample : N2485-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

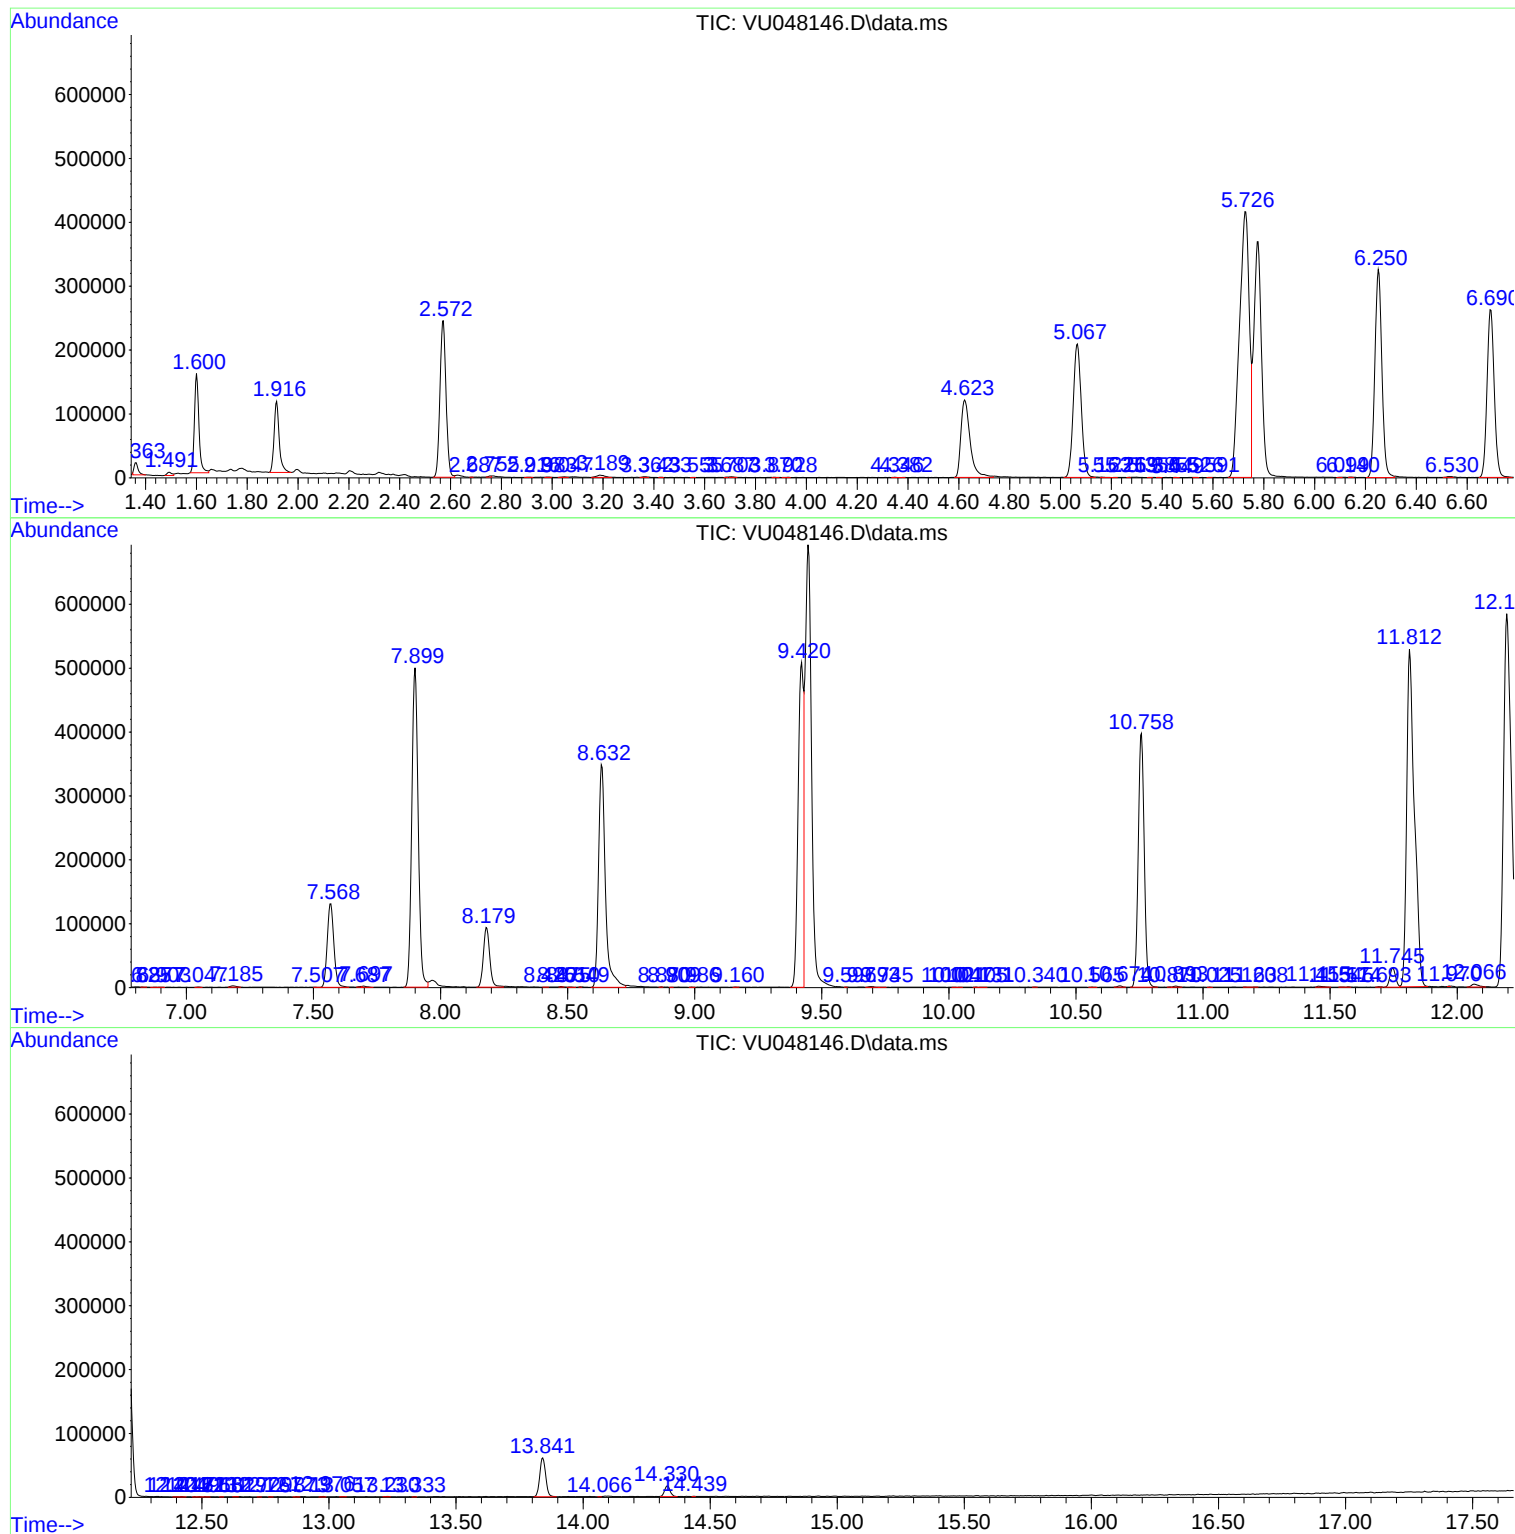

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048146.D
Acq On : 20 Apr 2022 16:32
Operator : SY/MD
Sample : N2485-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048146.D
Acq On : 20 Apr 2022 16:32
Operator : SY/MD
Sample : N2485-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc