

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048147.D
 Acq On : 20 Apr 2022 16:55
 Operator : SY/MD
 Sample : N2485-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	103	rBV	145682	171713	14.66%	1.837%
2	1.915	171	179	196	rVB	115652	158174	13.51%	1.693%
3	2.497	356	360	361	rBV2	451	284	0.02%	0.003%
4	2.571	369	383	398	rBV	242984	405297	34.60%	4.337%
5	2.694	418	421	426	rVB2	348	306	0.03%	0.003%
6	2.742	432	436	441	rVB3	459	395	0.03%	0.004%
7	2.864	471	474	479	rBV3	242	254	0.02%	0.003%
8	2.948	497	500	502	rBV2	358	223	0.02%	0.002%
9	3.047	525	531	538	rBV4	632	943	0.08%	0.010%
10	3.079	538	541	548	rVB2	489	426	0.04%	0.005%
11	3.115	548	552	555	rBV3	293	290	0.02%	0.003%
12	3.186	570	574	579	rBV2	248	276	0.02%	0.003%
13	3.311	609	613	614	rBV	340	248	0.02%	0.003%
14	3.600	699	703	706	rBV2	258	212	0.02%	0.002%
15	3.806	763	767	771	rBV	240	229	0.02%	0.002%
16	3.883	787	791	796	rVB2	475	467	0.04%	0.005%
17	4.568	996	1004	1007	rBV	324	345	0.03%	0.004%
18	4.626	1009	1022	1063	rBV2	119924	312915	26.72%	3.348%
19	5.066	1142	1159	1183	rVV	213184	467276	39.90%	5.000%
20	5.256	1214	1218	1223	rVB2	271	221	0.02%	0.002%
21	5.295	1223	1230	1236	rBV3	642	1062	0.09%	0.011%
22	5.337	1239	1243	1249	rVB2	260	238	0.02%	0.003%
23	5.365	1249	1252	1254	rBV2	293	190	0.02%	0.002%
24	5.452	1276	1279	1284	rVB2	229	188	0.02%	0.002%
25	5.497	1290	1293	1296	rBV	291	236	0.02%	0.003%
26	5.523	1296	1301	1302	rBV2	382	269	0.02%	0.003%
27	5.726	1339	1364	1394	rBV2	430640	1171211	100.00%	12.532%
28	5.989	1444	1446	1455	rVB3	539	604	0.05%	0.006%
29	6.050	1459	1465	1468	rVB3	529	553	0.05%	0.006%
30	6.115	1480	1485	1487	rBV2	237	203	0.02%	0.002%
31	6.150	1491	1496	1499	rBV3	222	210	0.02%	0.002%
32	6.182	1503	1506	1512	rVB2	274	201	0.02%	0.002%
33	6.250	1512	1527	1560	rBV	346115	660393	56.39%	7.066%
34	6.394	1571	1572	1579	rVB2	348	268	0.02%	0.003%
35	6.533	1604	1615	1622	rBV5	1804	3532	0.30%	0.038%
36	6.578	1626	1629	1635	rVB4	516	477	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048147.D
 Acq On : 20 Apr 2022 16:55
 Operator : SY/MD
 Sample : N2485-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.693	1650	1665	1683	rBV	270157	528501	45.12%	5.655%
38	6.973	1746	1752	1754	rBV	277	246	0.02%	0.003%
39	7.037	1769	1772	1774	rBV2	339	229	0.02%	0.002%
40	7.115	1793	1796	1801	rVB2	476	360	0.03%	0.004%
41	7.185	1808	1818	1829	rBV5	2413	4355	0.37%	0.047%
42	7.568	1922	1937	1957	rBV	132462	241115	20.59%	2.580%
43	7.684	1968	1973	1974	rBV3	634	522	0.04%	0.006%
44	7.787	2001	2005	2007	rBV2	459	389	0.03%	0.004%
45	7.899	2026	2040	2056	rBV	507125	891676	76.13%	9.541%
46	8.179	2116	2127	2150	rBV	95543	166133	14.18%	1.778%
47	8.504	2226	2228	2234	rVB4	487	422	0.04%	0.005%
48	8.552	2238	2243	2252	rVB5	1140	1481	0.13%	0.016%
49	8.635	2256	2269	2303	rBV	379067	706354	60.31%	7.558%
50	8.809	2321	2323	2328	rVB5	566	467	0.04%	0.005%
51	8.841	2328	2333	2339	rVB4	313	374	0.03%	0.004%
52	8.912	2350	2355	2357	rBV3	461	321	0.03%	0.003%
53	8.928	2357	2360	2364	rVB3	533	359	0.03%	0.004%
54	9.057	2396	2400	2405	rVB3	356	317	0.03%	0.003%
55	9.092	2405	2411	2415	rBV2	126	172	0.01%	0.002%
56	9.205	2442	2446	2449	rBV2	303	270	0.02%	0.003%
57	9.240	2455	2457	2461	rVB2	363	247	0.02%	0.003%
58	9.417	2497	2512	2547	rBV	507448	916940	78.29%	9.812%
59	9.571	2554	2560	2562	rBV5	817	723	0.06%	0.008%
60	9.697	2592	2599	2604	rBV3	1333	1684	0.14%	0.018%
61	9.751	2612	2616	2619	rVB	321	185	0.02%	0.002%
62	9.877	2653	2655	2660	rVB2	321	195	0.02%	0.002%
63	9.906	2660	2664	2666	rBV2	240	206	0.02%	0.002%
64	10.102	2717	2725	2728	rBV3	749	1077	0.09%	0.012%
65	10.288	2777	2783	2786	rBV2	447	580	0.05%	0.006%
66	10.484	2837	2844	2851	rBV3	420	719	0.06%	0.008%
67	10.671	2896	2902	2909	rVB5	2316	2825	0.24%	0.030%
68	10.758	2909	2929	2949	rBV	406508	672879	57.45%	7.200%
69	10.864	2959	2962	2964	rBV2	422	282	0.02%	0.003%
70	10.896	2964	2972	2978	rVV5	1022	1291	0.11%	0.014%
71	11.021	3008	3011	3017	rBV2	217	186	0.02%	0.002%
72	11.092	3027	3033	3039	rVB3	586	607	0.05%	0.006%
73	11.118	3039	3041	3042	rBV	473	177	0.02%	0.002%
74	11.172	3055	3058	3063	rBV3	188	184	0.02%	0.002%
75	11.259	3082	3085	3088	rBV2	273	217	0.02%	0.002%
76	11.323	3102	3105	3113	rVB	319	292	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048147.D
 Acq On : 20 Apr 2022 16:55
 Operator : SY/MD
 Sample : N2485-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.397	3126	3128	3135	rVB	269	254	0.02%	0.003%
78	11.436	3135	3140	3142	rBV2	415	346	0.03%	0.004%
79	11.465	3142	3149	3156	rBV5	1289	1910	0.16%	0.020%
80	11.555	3174	3177	3181	rBV	233	185	0.02%	0.002%
81	11.745	3229	3236	3244	rBV4	2570	3444	0.29%	0.037%
82	11.812	3244	3257	3276	rBV	534481	878055	74.97%	9.396%
83	11.899	3282	3284	3291	rVB3	389	294	0.03%	0.003%
84	11.970	3303	3306	3316	rVB7	1418	1585	0.14%	0.017%
85	12.066	3326	3336	3351	rBV3	10971	20231	1.73%	0.216%
86	12.192	3362	3375	3394	rBV	532715	893808	76.31%	9.564%
87	12.481	3461	3465	3469	rBV3	318	327	0.03%	0.003%
88	12.520	3474	3477	3480	rBV	264	199	0.02%	0.002%
89	12.597	3498	3501	3503	rBV2	339	179	0.02%	0.002%
90	12.639	3512	3514	3520	rVB4	310	305	0.03%	0.003%
91	12.693	3527	3531	3535	rBV4	335	306	0.03%	0.003%
92	12.735	3539	3544	3547	rVV3	346	365	0.03%	0.004%
93	12.767	3551	3554	3557	rVB2	366	254	0.02%	0.003%
94	13.102	3655	3658	3661	rBV	299	294	0.03%	0.003%
95	13.253	3702	3705	3708	rBV	397	279	0.02%	0.003%
96	13.339	3729	3732	3736	rBV2	359	285	0.02%	0.003%
97	13.844	3880	3889	3904	rBV2	12302	19567	1.67%	0.209%
98	14.333	4034	4041	4053	rVB5	4810	7472	0.64%	0.080%
99	14.597	4120	4123	4127	rBV3	464	335	0.03%	0.004%
100	15.999	4553	4559	4571	rVB4	6400	9263	0.79%	0.099%




Sum of corrected areas: 9345430

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048147.D
Acq On : 20 Apr 2022 16:55
Operator : SY/MD
Sample : N2485-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

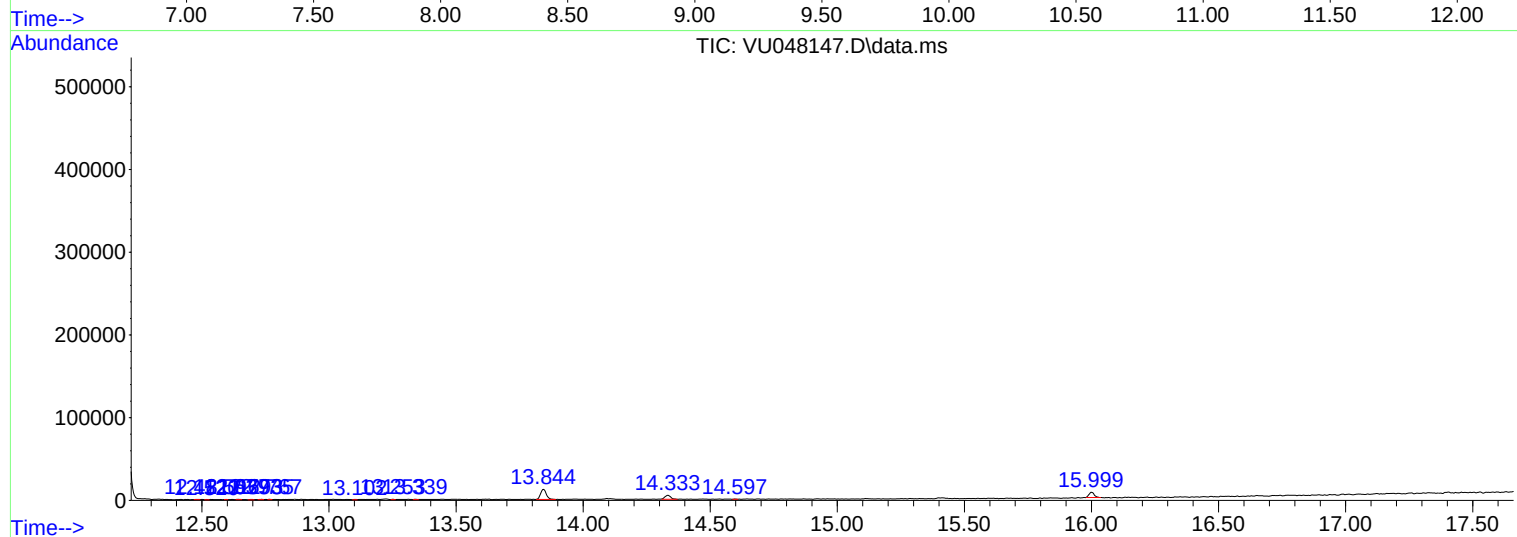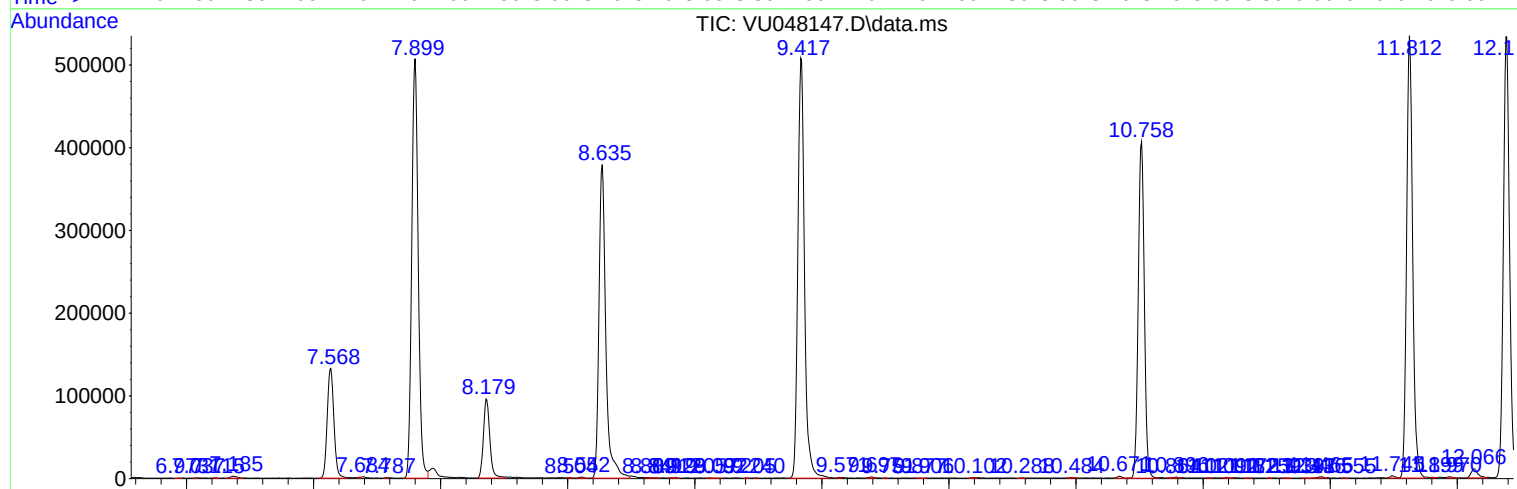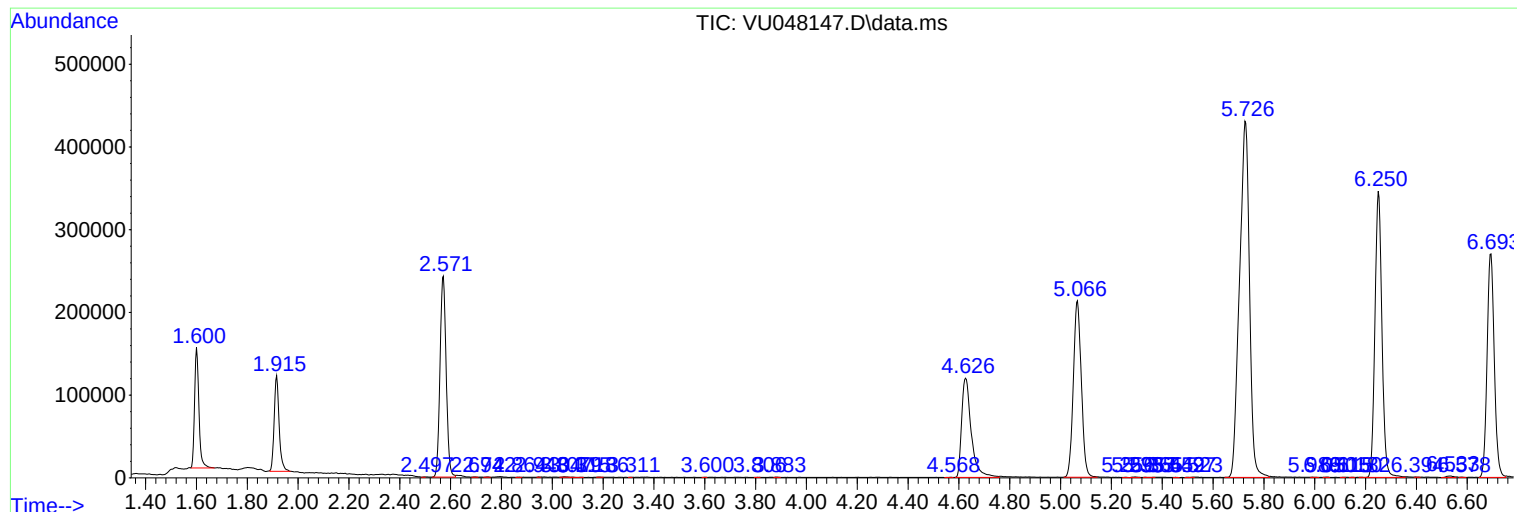

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048147.D
Acq On : 20 Apr 2022 16:55
Operator : SY/MD
Sample : N2485-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048147.D
Acq On : 20 Apr 2022 16:55
Operator : SY/MD
Sample : N2485-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc