

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048159.D
 Acq On : 20 Apr 2022 21:32
 Operator : SY/MD
 Sample : VIBLK063
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048159.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	147893	179826	11.44%	1.578%
2	1.916	171	179	198	rVB	119088	165886	10.55%	1.456%
3	2.568	370	382	399	rBV	253934	426532	27.13%	3.744%
4	2.729	429	432	436	rVB3	347	264	0.02%	0.002%
5	2.790	442	451	454	rBV6	1471	2318	0.15%	0.020%
6	2.967	497	506	510	rBV5	539	958	0.06%	0.008%
7	3.051	521	532	546	rBV	9525	18884	1.20%	0.166%
8	3.189	558	575	594	rBV2	8524	19037	1.21%	0.167%
9	3.256	594	596	602	rVB3	360	346	0.02%	0.003%
10	3.301	606	610	613	rBV3	296	310	0.02%	0.003%
11	3.539	682	684	689	rVB2	333	259	0.02%	0.002%
12	3.578	689	696	699	rBV2	359	398	0.03%	0.003%
13	3.655	715	720	721	rBV	315	256	0.02%	0.002%
14	3.774	754	757	762	rVB2	379	298	0.02%	0.003%
15	3.797	762	764	767	rBV	339	224	0.01%	0.002%
16	3.848	776	780	781	rBV	449	302	0.02%	0.003%
17	4.031	835	837	841	rVV	339	227	0.01%	0.002%
18	4.202	885	890	897	rVB3	478	516	0.03%	0.005%
19	4.253	897	906	912	rBV3	532	813	0.05%	0.007%
20	4.285	912	916	920	rVV3	358	307	0.02%	0.003%
21	4.575	1003	1006	1008	rBV	352	259	0.02%	0.002%
22	4.626	1009	1022	1061	rBV2	144871	379497	24.14%	3.331%
23	4.870	1094	1098	1101	rBV2	316	276	0.02%	0.002%
24	5.067	1142	1159	1178	rBV	219210	484279	30.81%	4.251%
25	5.292	1223	1229	1232	rBV4	699	800	0.05%	0.007%
26	5.350	1240	1247	1253	rVB3	390	490	0.03%	0.004%
27	5.382	1253	1257	1261	rBV2	396	364	0.02%	0.003%
28	5.452	1277	1279	1282	rBV2	284	215	0.01%	0.002%
29	5.469	1282	1284	1287	rVB2	409	237	0.02%	0.002%
30	5.581	1317	1319	1326	rVB3	356	356	0.02%	0.003%
31	5.726	1343	1364	1376	rBV2	460592	1254801	79.82%	11.014%
32	5.919	1421	1424	1428	rBV4	291	245	0.02%	0.002%
33	5.977	1440	1442	1445	rBV2	354	222	0.01%	0.002%
34	6.038	1457	1461	1466	rVB3	602	555	0.04%	0.005%
35	6.102	1478	1481	1483	rBV3	352	234	0.01%	0.002%
36	6.118	1483	1486	1489	rBV2	411	272	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048159.D
 Acq On : 20 Apr 2022 21:32
 Operator : SY/MD
 Sample : VIBLK063
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1508	1527	1551	rBV	434323	843186	53.64%	7.401%
38	6.530	1607	1614	1629	rBV9	2111	3984	0.25%	0.035%
39	6.694	1650	1665	1688	rBV	281943	556073	35.37%	4.881%
40	6.841	1708	1711	1713	rBV2	391	234	0.01%	0.002%
41	6.948	1742	1744	1749	rBV	313	273	0.02%	0.002%
42	7.050	1772	1776	1780	rVB2	441	394	0.03%	0.003%
43	7.185	1809	1818	1825	rBV4	2639	4398	0.28%	0.039%
44	7.517	1916	1921	1924	rBV3	352	337	0.02%	0.003%
45	7.565	1924	1936	1964	rBV	145256	261661	16.65%	2.297%
46	7.690	1966	1975	1986	rVB4	1945	3516	0.22%	0.031%
47	7.790	2002	2006	2014	rBV5	746	887	0.06%	0.008%
48	7.899	2023	2040	2056	rBV	558316	976456	62.12%	8.570%
49	8.182	2116	2128	2147	rBV	99867	173901	11.06%	1.526%
50	8.423	2199	2203	2205	rBV2	474	306	0.02%	0.003%
51	8.636	2255	2269	2298	rBV	410349	751621	47.81%	6.597%
52	8.854	2332	2337	2339	rBV3	332	312	0.02%	0.003%
53	8.922	2348	2358	2360	rBV5	1346	1761	0.11%	0.015%
54	9.099	2410	2413	2416	rVV2	301	214	0.01%	0.002%
55	9.137	2421	2425	2427	rBV3	351	218	0.01%	0.002%
56	9.163	2427	2433	2440	rVB3	373	557	0.04%	0.005%
57	9.314	2476	2480	2486	rVB2	422	333	0.02%	0.003%
58	9.362	2491	2495	2498	rBV3	468	394	0.03%	0.003%
59	9.417	2498	2512	2518	rBV	637982	1130770	71.93%	9.925%
60	9.610	2567	2572	2573	rBV2	461	318	0.02%	0.003%
61	9.642	2579	2582	2585	rBV2	528	414	0.03%	0.004%
62	9.690	2594	2597	2604	rVV4	854	1003	0.06%	0.009%
63	9.780	2623	2625	2627	rBV	371	223	0.01%	0.002%
64	9.944	2672	2676	2679	rVV2	491	338	0.02%	0.003%
65	9.967	2679	2683	2688	rVB3	348	301	0.02%	0.003%
66	10.102	2722	2725	2728	rVB2	472	344	0.02%	0.003%
67	10.365	2804	2807	2813	rVB2	295	272	0.02%	0.002%
68	10.446	2827	2832	2835	rBV2	349	317	0.02%	0.003%
69	10.549	2860	2864	2867	rVV2	405	332	0.02%	0.003%
70	10.626	2881	2888	2891	rBV3	356	452	0.03%	0.004%
71	10.668	2894	2901	2909	rVV4	2503	3184	0.20%	0.028%
72	10.758	2916	2929	2946	rBV	425943	687328	43.72%	6.033%
73	10.861	2954	2961	2962	rBV2	528	495	0.03%	0.004%
74	10.951	2985	2989	2994	rBV3	401	397	0.03%	0.003%
75	11.115	3039	3040	3044	rVB2	404	275	0.02%	0.002%
76	11.150	3048	3051	3056	rVB3	490	391	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
 Data File : VU048159.D
 Acq On : 20 Apr 2022 21:32
 Operator : SY/MD
 Sample : VIBLK063
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.224	3071	3074	3078	rVB3	495	422	0.03%	0.004%
78	11.272	3085	3089	3091	rBV2	259	222	0.01%	0.002%
79	11.298	3094	3097	3100	rBV2	286	216	0.01%	0.002%
80	11.317	3100	3103	3107	rBV2	276	218	0.01%	0.002%
81	11.459	3139	3147	3148	rBV3	1371	1641	0.10%	0.014%
82	11.523	3162	3167	3172	rBV2	237	299	0.02%	0.003%
83	11.652	3204	3207	3214	rVB2	333	317	0.02%	0.003%
84	11.697	3214	3221	3225	rBV4	1085	1165	0.07%	0.010%
85	11.745	3225	3236	3245	rBV2	17552	27834	1.77%	0.244%
86	11.812	3245	3257	3283	rVB2	702233	1572005	100.00%	13.798%
87	12.031	3323	3325	3327	rBV	405	226	0.01%	0.002%
88	12.079	3334	3340	3344	rVB5	969	1412	0.09%	0.012%
89	12.195	3358	3376	3400	rBV3	637393	1335572	84.96%	11.723%
90	12.639	3509	3514	3523	rVB4	667	781	0.05%	0.007%
91	12.677	3523	3526	3529	rBV3	313	259	0.02%	0.002%
92	12.999	3621	3626	3627	rBV2	365	312	0.02%	0.003%
93	13.153	3671	3674	3677	rBV2	360	240	0.02%	0.002%
94	13.475	3771	3774	3780	rBV3	389	413	0.03%	0.004%
95	13.523	3786	3789	3793	rBV2	307	277	0.02%	0.002%
96	13.584	3805	3808	3812	rBV2	337	240	0.02%	0.002%
97	13.841	3878	3888	3903	rBV	47748	77033	4.90%	0.676%
98	13.973	3924	3929	3934	rBV3	565	742	0.05%	0.007%
99	14.250	4012	4015	4018	rBV	387	292	0.02%	0.003%
100	14.330	4030	4040	4051	rBV3	13491	21863	1.39%	0.192%




Sum of corrected areas: 11393234

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048159.D
Acq On : 20 Apr 2022 21:32
Operator : SY/MD
Sample : VIBLK063
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK063

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

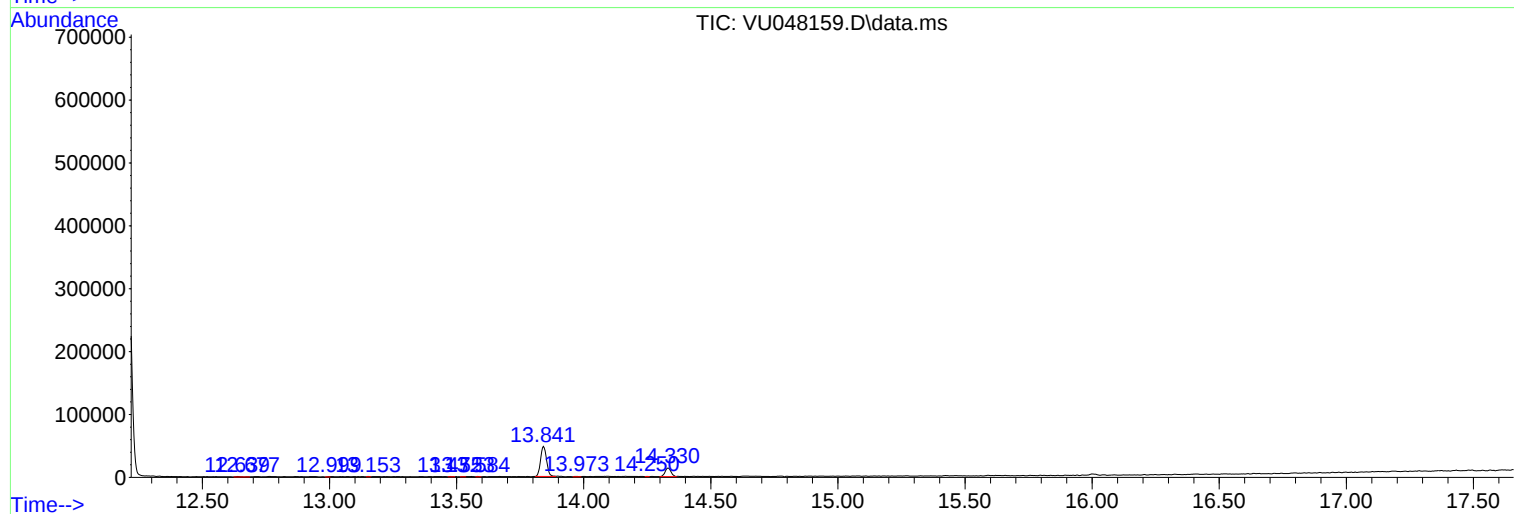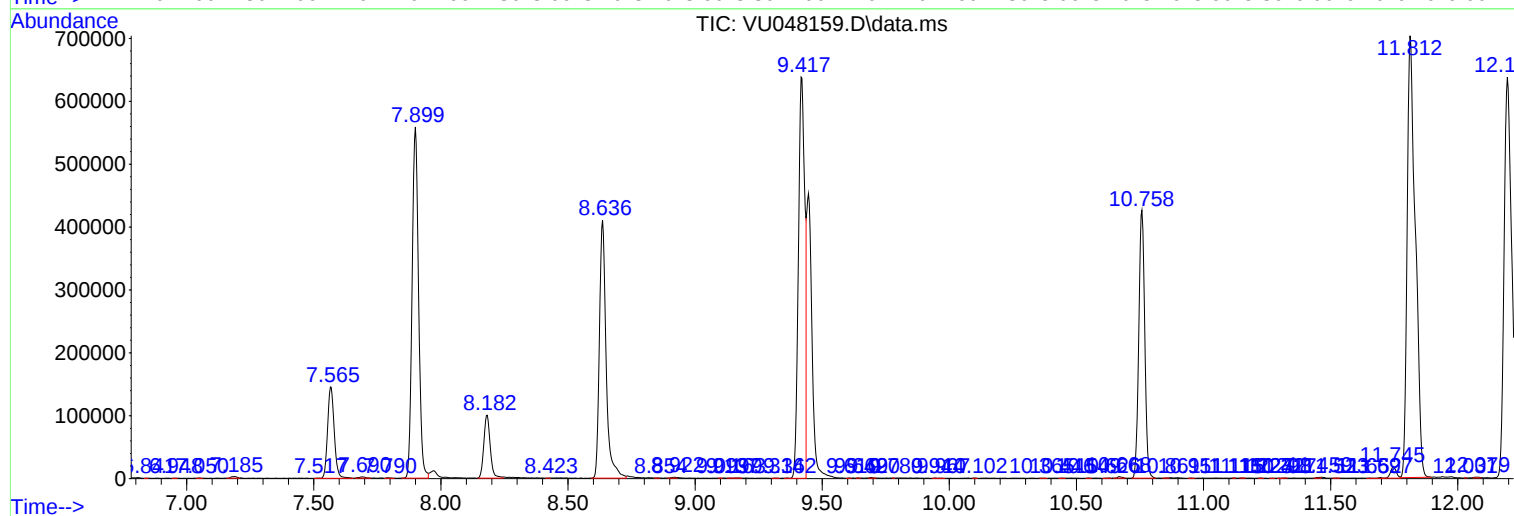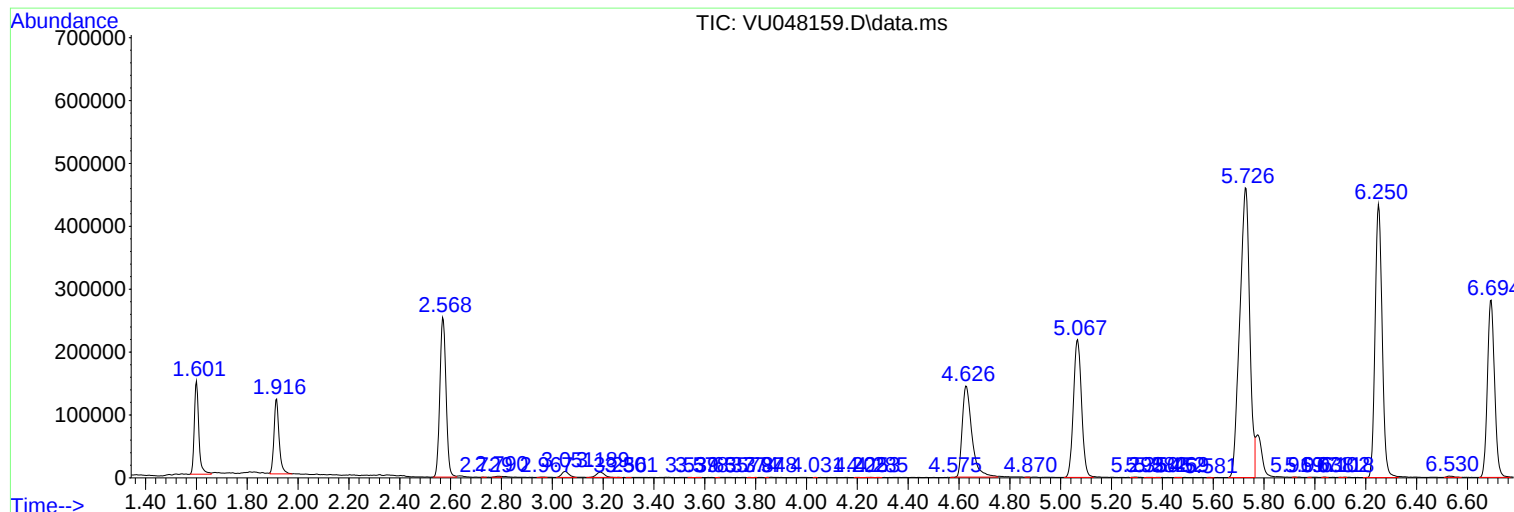

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048159.D
Acq On : 20 Apr 2022 21:32
Operator : SY/MD
Sample : VIBLK063
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK063

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048159.D
Acq On : 20 Apr 2022 21:32
Operator : SY/MD
Sample : VIBLK063
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK063

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
