


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042022\
Data File : VU048137.D
Acq On : 20 Apr 2022 12:11
Operator : SY/MD
Sample : BFB068
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB068

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Title : VOC Analysis
Last Update : Mon Apr 25 01:24:32 2022

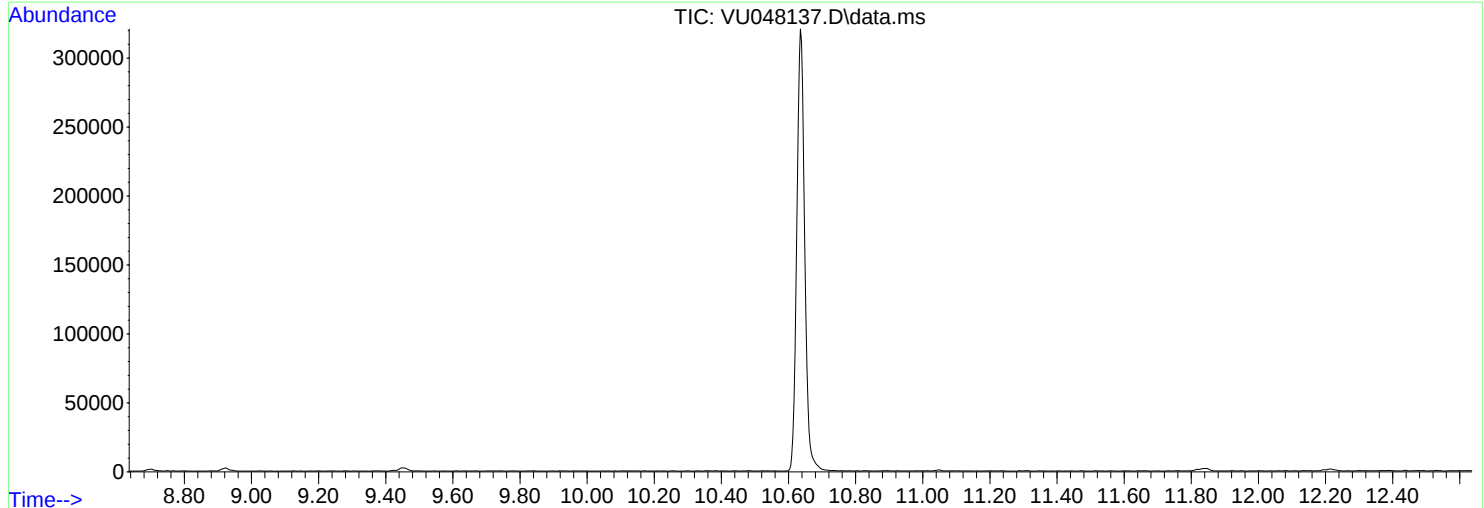

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	10337	PASS
75	95	30	80	47.3	29189	PASS
95	95	100	100	100.0	61749	PASS
96	95	5	9	6.9	4271	PASS
173	174	0.00	2	1.4	802	PASS
174	95	50	120	93.1	57483	PASS
175	174	5	9	7.4	4252	PASS
176	174	95	101	95.8	55061	PASS
177	176	5	9	7.0	3833	PASS

m/z	Abundance
39.90	321.0
43.90	436.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
36.00	492.0
37.00	2212.0
37.90	2063.0
39.00	1152.0
39.90	313.0
43.90	749.0
45.00	427.0
46.90	524.0
47.90	423.0
49.00	2146.0
50.00	10360.0
51.00	3373.0
52.00	144.0
55.10	138.0
55.90	705.0
57.00	1680.0
60.00	537.0
61.00	2693.0
62.00	2926.0
63.00	2568.0
64.00	564.0
65.10	646.0
66.80	136.0
68.00	5711.0
69.00	6198.0
69.90	360.0
72.00	269.0
73.00	2497.0
74.00	9219.0
75.00	28568.0
76.00	2369.0
76.90	360.0
77.90	254.0
78.90	2181.0
79.90	763.0
80.90	2348.0
81.90	702.0
86.00	107.0
87.00	2551.0
87.90	2598.0
91.00	267.0
92.00	1658.0
93.00	2695.0
94.00	6667.0
95.00	60216.0
96.00	4313.0
97.10	185.0
103.80	224.0
104.90	110.0
106.00	237.0
106.90	102.0
115.80	208.0
116.80	493.0
117.80	259.0
118.80	354.0
127.90	188.0
129.90	211.0
130.90	104.0
134.90	135.0
140.90	527.0
142.90	823.0
144.90	370.0
146.00	108.0
147.80	222.0
154.90	150.0
171.00	167.0
171.90	1084.0
173.00	766.0
173.90	54288.0
175.00	3967.0
175.90	51928.0
176.90	3557.0
206.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
36.00	460.0
37.00	2277.0
38.00	2194.0
39.00	1063.0
39.90	336.0
43.90	873.0
44.90	415.0
46.90	734.0
48.00	439.0
49.00	2277.0
50.00	10640.0
51.00	3450.0
52.00	159.0
55.00	171.0
55.90	766.0
57.00	1648.0
60.00	576.0
61.00	2938.0
62.00	3037.0
63.00	2708.0
64.00	503.0
65.10	653.0
66.90	125.0
68.00	6005.0
69.00	6499.0
69.90	355.0
71.90	244.0
73.00	2596.0
74.00	9771.0
75.00	30144.0
76.00	2493.0
76.90	409.0
77.90	281.0
78.90	2362.0
79.90	745.0
80.90	2350.0
81.90	736.0
86.90	2718.0
87.90	2844.0
91.10	278.0
92.00	1818.0
93.00	2759.0
94.00	7145.0
95.00	63752.0
96.00	4460.0
97.10	157.0
103.80	263.0
104.90	119.0
106.00	291.0
115.80	220.0
116.80	538.0
117.80	247.0
118.80	388.0
127.90	205.0
129.90	240.0
134.90	163.0
140.90	628.0
141.90	103.0
142.90	902.0
144.90	438.0
145.80	116.0
147.80	198.0
154.80	143.0
170.90	195.0
171.90	1144.0
173.00	837.0
173.90	59344.0
175.00	4407.0
175.90	56560.0
176.90	4010.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068

m/z	Abundance
35.90	420.0
37.00	2319.0
38.00	2117.0
39.00	936.0
39.90	350.0
43.90	901.0
44.90	371.0
46.90	815.0
48.00	421.0
49.00	2198.0
50.00	10010.0
51.00	3163.0
52.00	141.0
55.00	194.0
55.90	807.0
57.00	1454.0
60.00	545.0
61.00	2838.0
62.00	2835.0
63.00	2602.0
64.00	374.0
65.10	586.0
65.90	103.0
67.10	154.0
68.00	5680.0
69.00	6002.0
69.90	359.0
71.90	198.0
73.00	2467.0
74.00	9530.0
75.00	28856.0
76.00	2448.0
76.90	403.0
77.90	288.0
78.90	2305.0
79.90	679.0
80.90	2118.0
81.90	653.0
86.90	2673.0
88.00	2775.0
91.00	253.0
92.00	1753.0
93.00	2538.0
94.00	6976.0
95.00	61280.0
96.00	4040.0
97.00	137.0
103.80	288.0
105.90	288.0
115.80	199.0
116.80	561.0
117.80	208.0
118.80	406.0
127.90	164.0
129.90	215.0
134.90	156.0
140.90	646.0
142.90	907.0
144.90	444.0
145.80	122.0
147.80	133.0
154.80	150.0
170.90	201.0
171.90	1028.0
173.10	803.0
173.90	58816.0
175.00	4382.0
175.90	56696.0
176.90	3931.0

Instrument :
MSVOA_U
ClientSampleId :
BFB068