

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
 Data File : VU053797.D
 Acq On : 20 Apr 2023 11:26
 Operator : JC/MD
 Sample : VU0420WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK186

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rVB	58006	69607	16.07%	1.919%
2	1.912	169	178	200	rVB	54100	75184	17.36%	2.073%
3	2.565	369	381	399	rBV	89791	146625	33.86%	4.043%
4	3.044	519	530	541	rVB	5845	10581	2.44%	0.292%
5	4.626	1010	1022	1050	rBV	56233	154330	35.64%	4.255%
6	5.057	1140	1156	1177	rVB2	85422	192963	44.56%	5.320%
7	5.719	1342	1362	1386	rBV2	165264	433040	100.00%	11.939%
8	6.243	1512	1525	1544	rBV	157272	299758	69.22%	8.265%
9	6.687	1647	1663	1681	rBV	105474	206182	47.61%	5.685%
10	7.562	1924	1935	1953	rBV	44668	80734	18.64%	2.226%
11	7.893	2025	2038	2059	rBV	201233	351962	81.28%	9.704%
12	8.179	2112	2127	2148	rVB2	27173	48239	11.14%	1.330%
13	8.629	2255	2267	2298	rBV	210954	395366	91.30%	10.901%
14	9.414	2498	2511	2537	rBV	215177	364955	84.28%	10.062%
15	10.751	2915	2927	2945	rVB	83183	131545	30.38%	3.627%
16	11.809	3244	3256	3273	rBV	211929	341941	78.96%	9.428%
17	12.189	3359	3374	3388	rBV2	188279	311669	71.97%	8.593%
18	13.844	3882	3889	3901	rBV4	3967	5988	1.38%	0.165%
19	14.330	4032	4040	4052	rBV6	4060	6360	1.47%	0.175%




Sum of corrected areas: 3627029

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053797.D
Acq On : 20 Apr 2023 11:26
Operator : JC/MD
Sample : VU0420WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK186

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

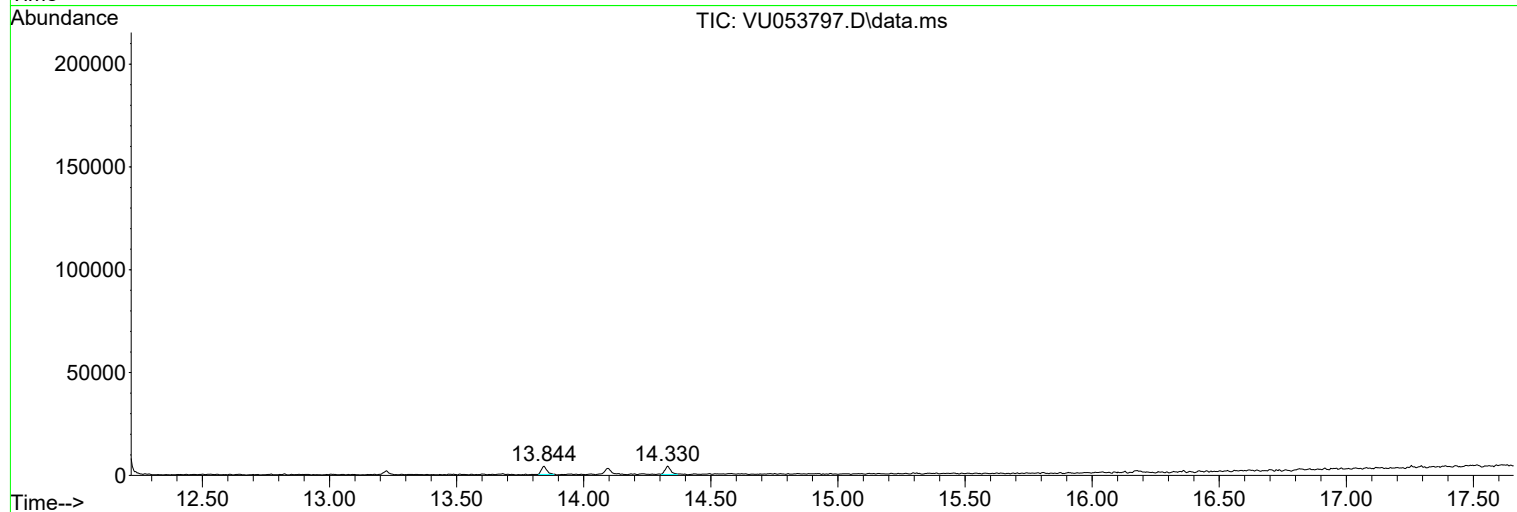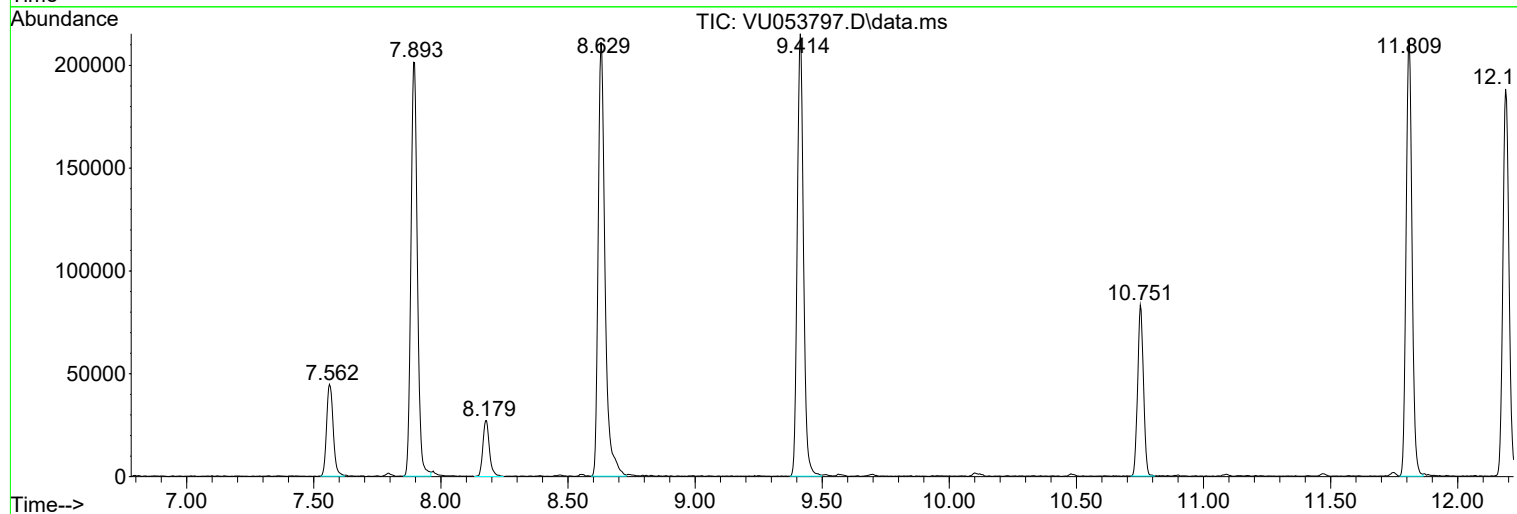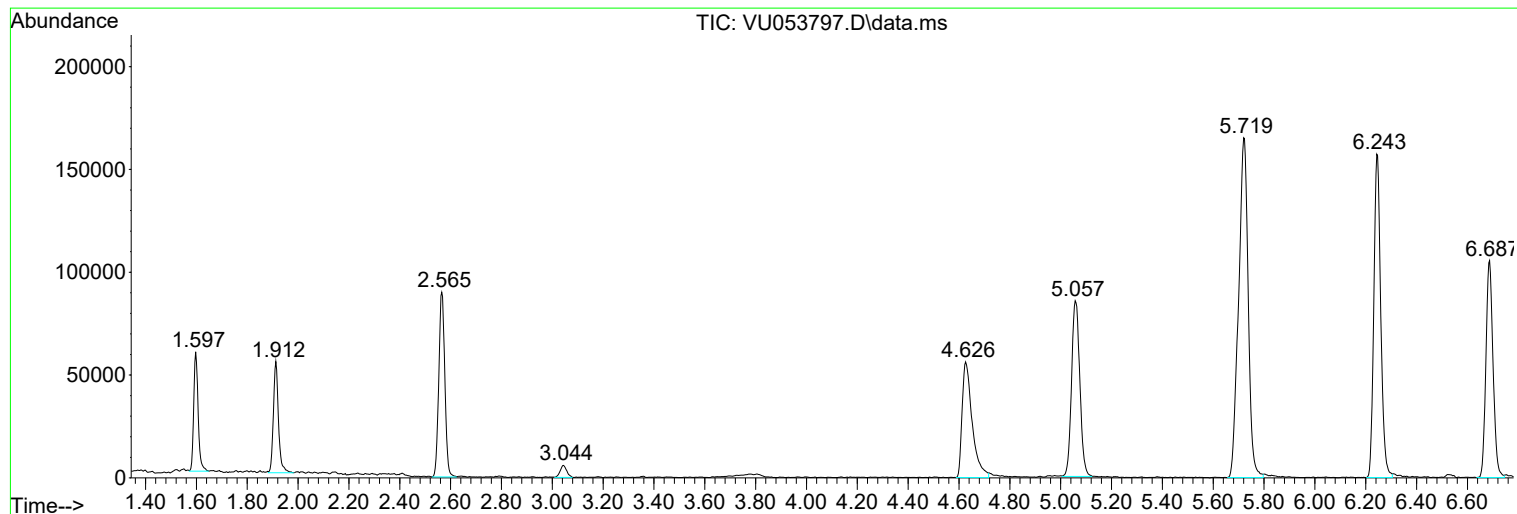

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053797.D
Acq On : 20 Apr 2023 11:26
Operator : JC/MD
Sample : VU0420WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK186

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042023\
Data File : VU053797.D
Acq On : 20 Apr 2023 11:26
Operator : JC/MD
Sample : VU0420WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK186

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc